




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023777.D
 Acq On : 24 Jan 2023 15:09
 Operator : CG/JU
 Sample : 01226-14
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9G1

Manual IntegrationsAPPROVED

Quant Time: Jan 24 23:57:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 24 23:52:16 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2023
 Supervised By :Yogesh Patel 01/25/2023

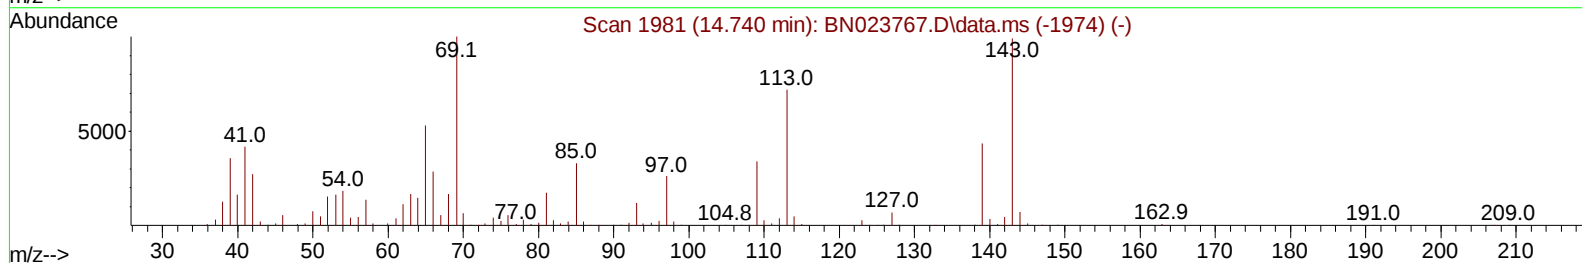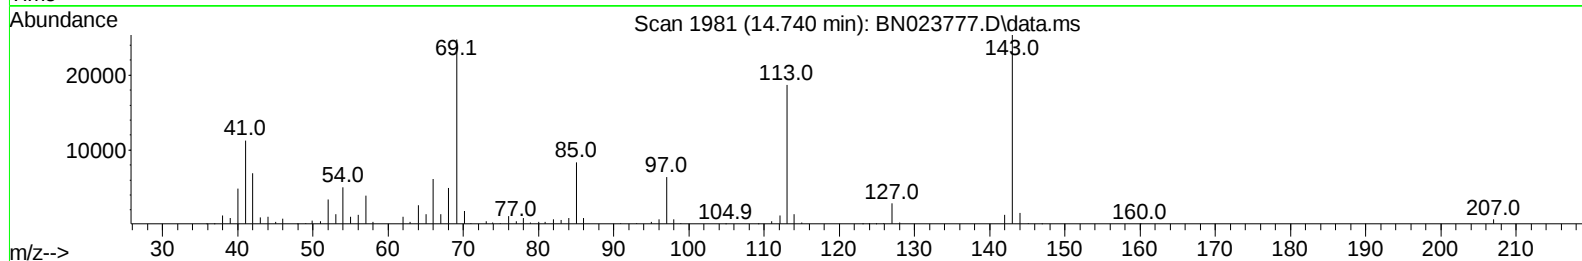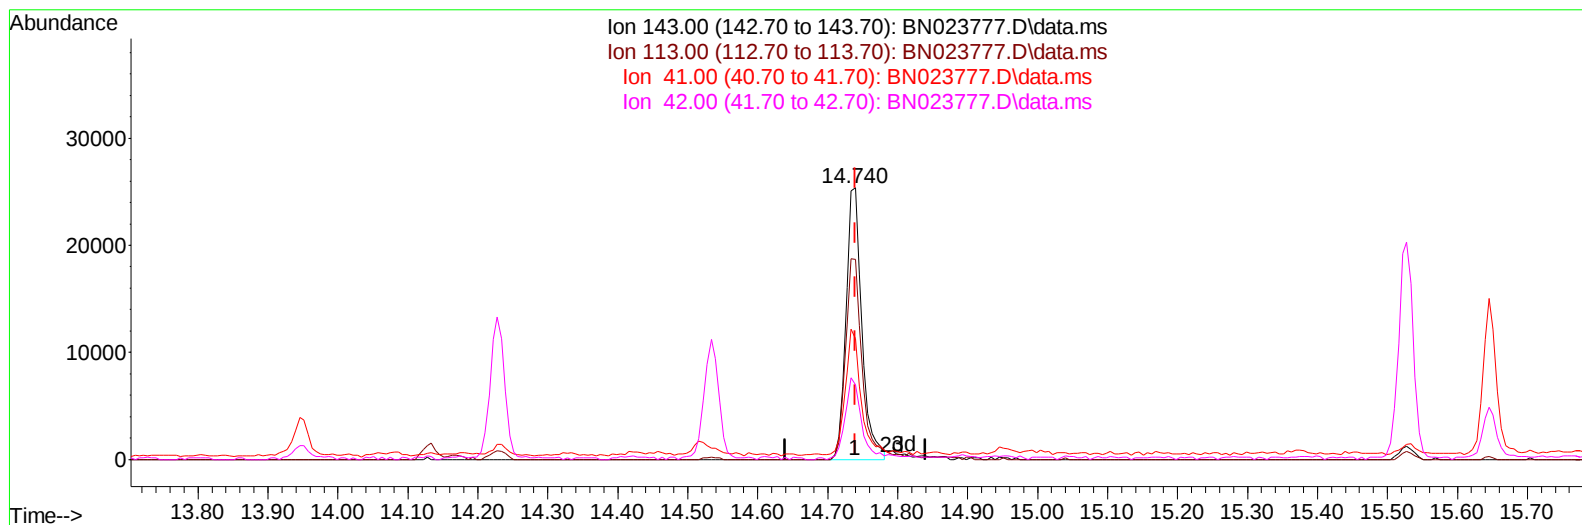

TIC: BN023777.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.740min (-0.000) 5.99 ng/u1

response 39685

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.00	73.79
41.00	40.90	44.53
42.00	27.80	27.41




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023777.D
Acq On : 24 Jan 2023 15:09
Operator : CG/JU
Sample : 01226-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9G1

Manual IntegrationsAPPROVED

Quant Time: Jan 24 23:57:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 24 23:52:16 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2023
Supervised By :Yogesh Patel 01/25/2023

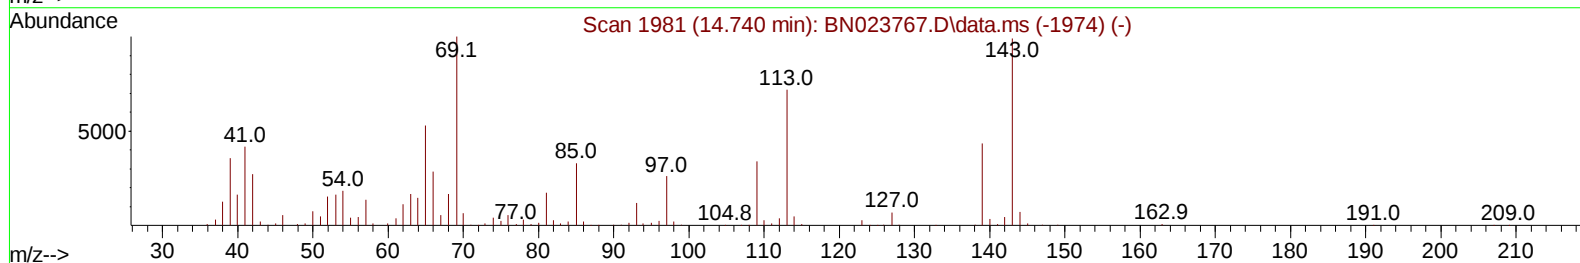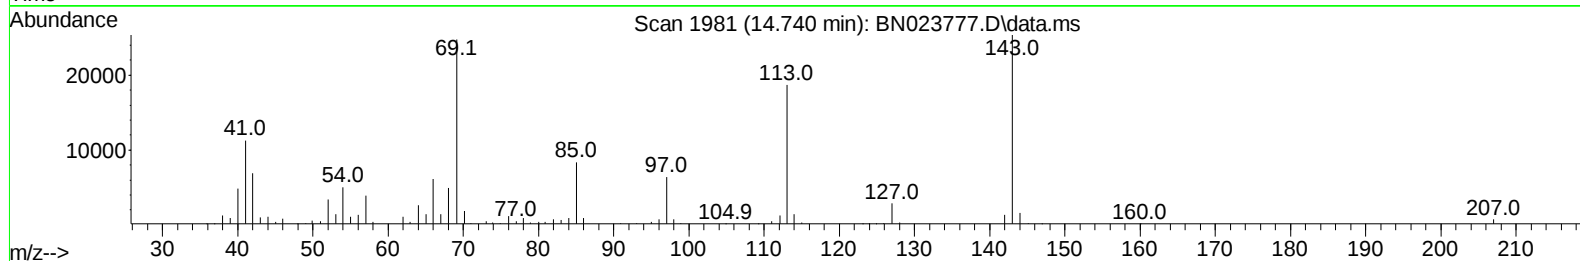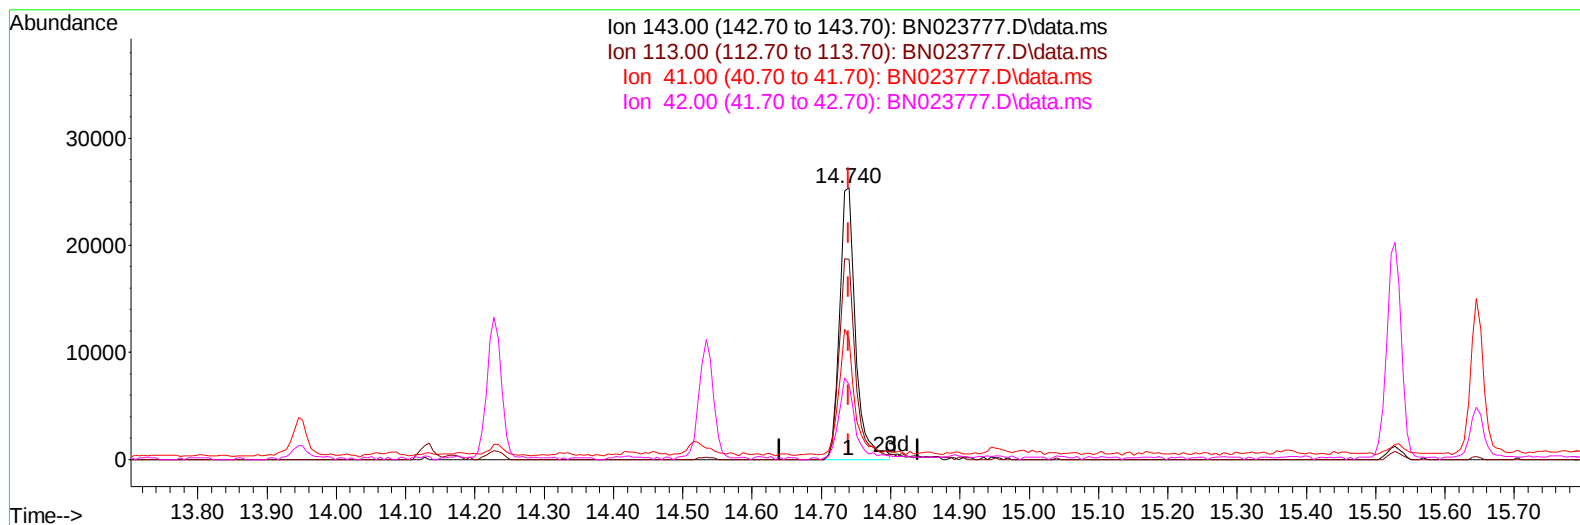

TIC: BN023777.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.740min (-0.000) 6.10 ng/ul m

response 40416

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.00	73.79
41.00	40.90	44.53
42.00	27.80	27.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023777.D
 Acq On : 24 Jan 2023 15:09
 Operator : CG/JU
 Sample : 01226-14
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/25/2023
 Supervised By :Yogesh Patel 01/25/2023

Quant Time: Jan 24 23:57:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 24 23:52:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	177958	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	711067	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	437429	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	947891	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	958393	20.000	ng/ul	0.00
88) Perylene-d12	23.880	264	1013276	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	19346	4.678	ng/uL	0.00
4) Pyridine-d5	3.699	84	110700	8.922	ng/ul	0.00
7) Phenol-d5	7.052	99	95112	6.030	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	287735	29.738	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132	281768	23.327	ng/ul	0.00
15) 4-Methylphenol-d8	8.599	113	183079	14.543	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	186111	34.710	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	190442	33.551	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	318066	29.378	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	426982	25.072	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1253861	38.533	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1329473	36.874	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	40416m	6.101	ng/ul	0.00
60) Fluorene-d10	15.528	176	1047122	37.660	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	193327	33.809	ng/ul	0.00
73) Anthracene-d10	17.381	188	1720083	40.552	ng/ul	0.00
81) Pyrene-d10	19.675	212	1880584	34.310	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	2074116	41.392	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023777.D
Acq On : 24 Jan 2023 15:09
Operator : CG/JU
Sample : 01226-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/25/2023
Supervised By :Yogesh Patel 01/25/2023

Quant Time: Jan 24 23:57:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 24 23:52:16 2023
Response via : Initial Calibration

