

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023750.D
 Acq On : 23 Jan 2023 13:32
 Operator : CG/JU
 Sample : 01146-14MEDL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

Quant Time: Jan 23 23:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	200839	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	798514	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	457592	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	931778	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	843794	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264	817913	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.052	99	8023	0.451	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	7383	0.676	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	6848	0.502	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	5285	0.372	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	2972	0.494	ng/ul	0.00
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.322	165	4382m	0.360	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	8444m	0.442	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	19554m	0.574	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	19078	0.506	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.528	176	17489	0.601	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.381	188	23313	0.559	ng/ul	0.00
81) Pyrene-d10	19.675	212	26579	0.551	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	20160	0.498	ng/ul	-0.03
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.386	149	935975	27.312	ng/ul#	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023750.D
Acq On : 23 Jan 2023 13:32
Operator : CG/JU
Sample : 01146-14MEDL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4462MEDL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023


Quant Time: Jan 23 23:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

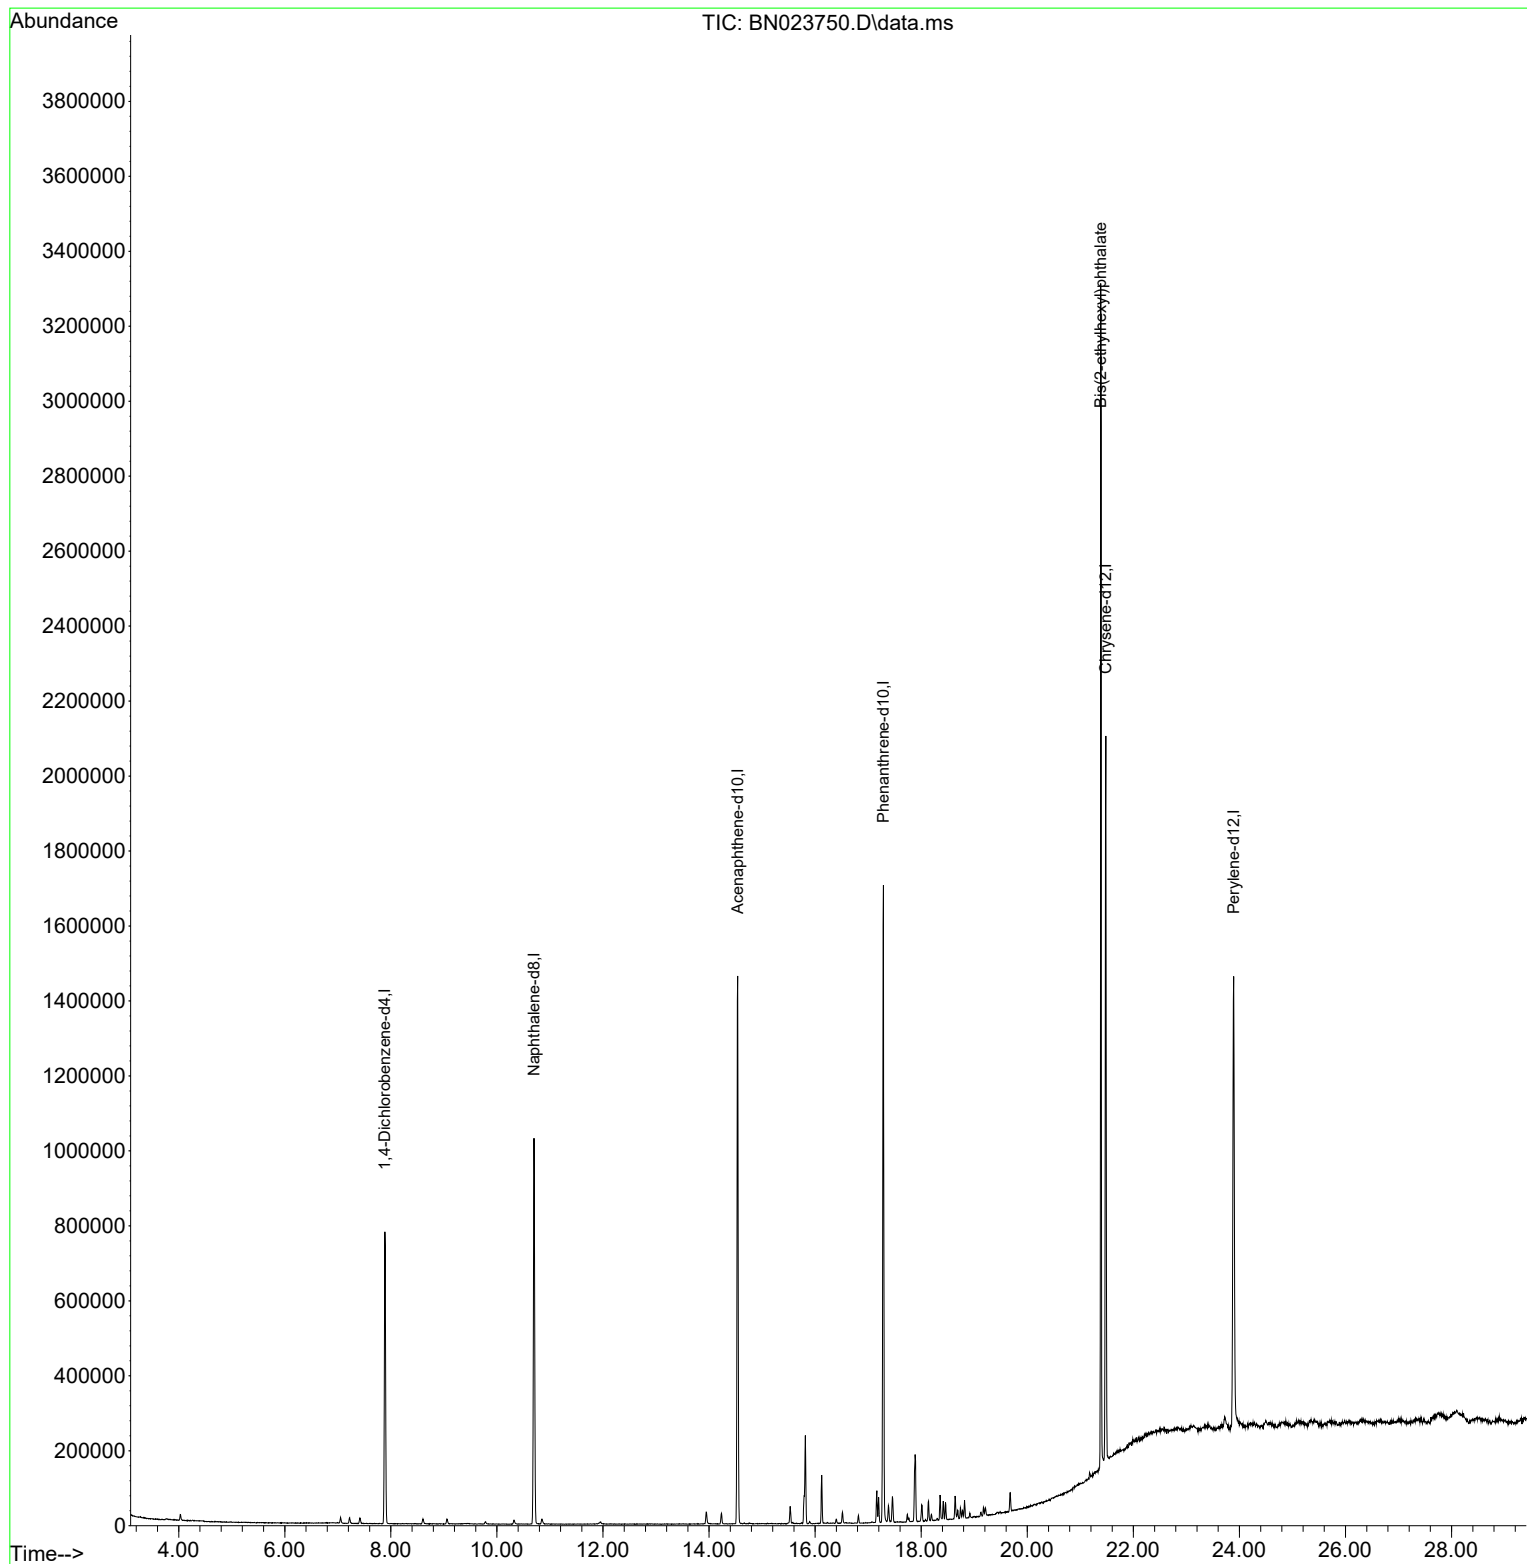

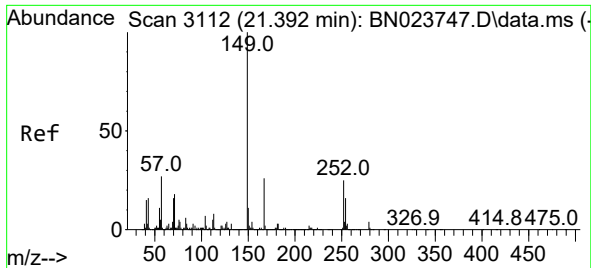

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 27.312 ng/ul
 RT: 21.386 min Scan# 3111
 Delta R.T. -0.006 min
 Lab File: BN023750.D
 Acq: 23 Jan 2023 13:32

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

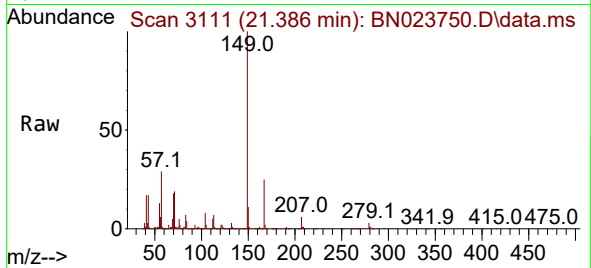

Tgt Ion:149 Resp: 935975
 Ion Ratio Lower Upper
 149 100
 167 24.9 22.0 33.0
 279 3.4 3.4 5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

