

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023761.D
 Acq On : 23 Jan 2023 20:34
 Operator : CG/JU
 Sample : 01226-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9F7

Quant Time: Jan 24 00:02:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	200616	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	850088	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	516015	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.281	188	1084496	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	1122729	20.000	ng/ul	-0.01
88) Perylene-d12	23.904	264	1298760	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	20639	4.427	ng/uL	0.00
4) Pyridine-d5	3.693	84	192449	13.759	ng/ul	0.00
7) Phenol-d5	7.052	99	106716	6.002	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	261399	23.965	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132	262566	19.282	ng/ul	0.00
15) 4-Methylphenol-d8	8.599	113	209326	14.750	ng/ul	-0.01
21) Nitrobenzene-d5	9.057	128	160366	25.017	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	171595	25.287	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	303365	23.438	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.840	131	507306	24.917	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	1068662	27.840	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1176787	27.669	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	33392	4.273	ng/ul	0.00
60) Fluorene-d10	15.528	176	799433	24.373	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	102773	15.709	ng/ul	0.00
73) Anthracene-d10	17.381	188	1410694	29.068	ng/ul	0.00
81) Pyrene-d10	19.680	212	1757041	27.364	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	1833013	28.539	ng/ul	-0.02
Target Compounds						
52) Acenaphthene	14.598	153	76160	2.284	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023761.D
Acq On : 23 Jan 2023 20:34
Operator : CG/JU
Sample : 01226-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9F7

Quant Time: Jan 24 00:02:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

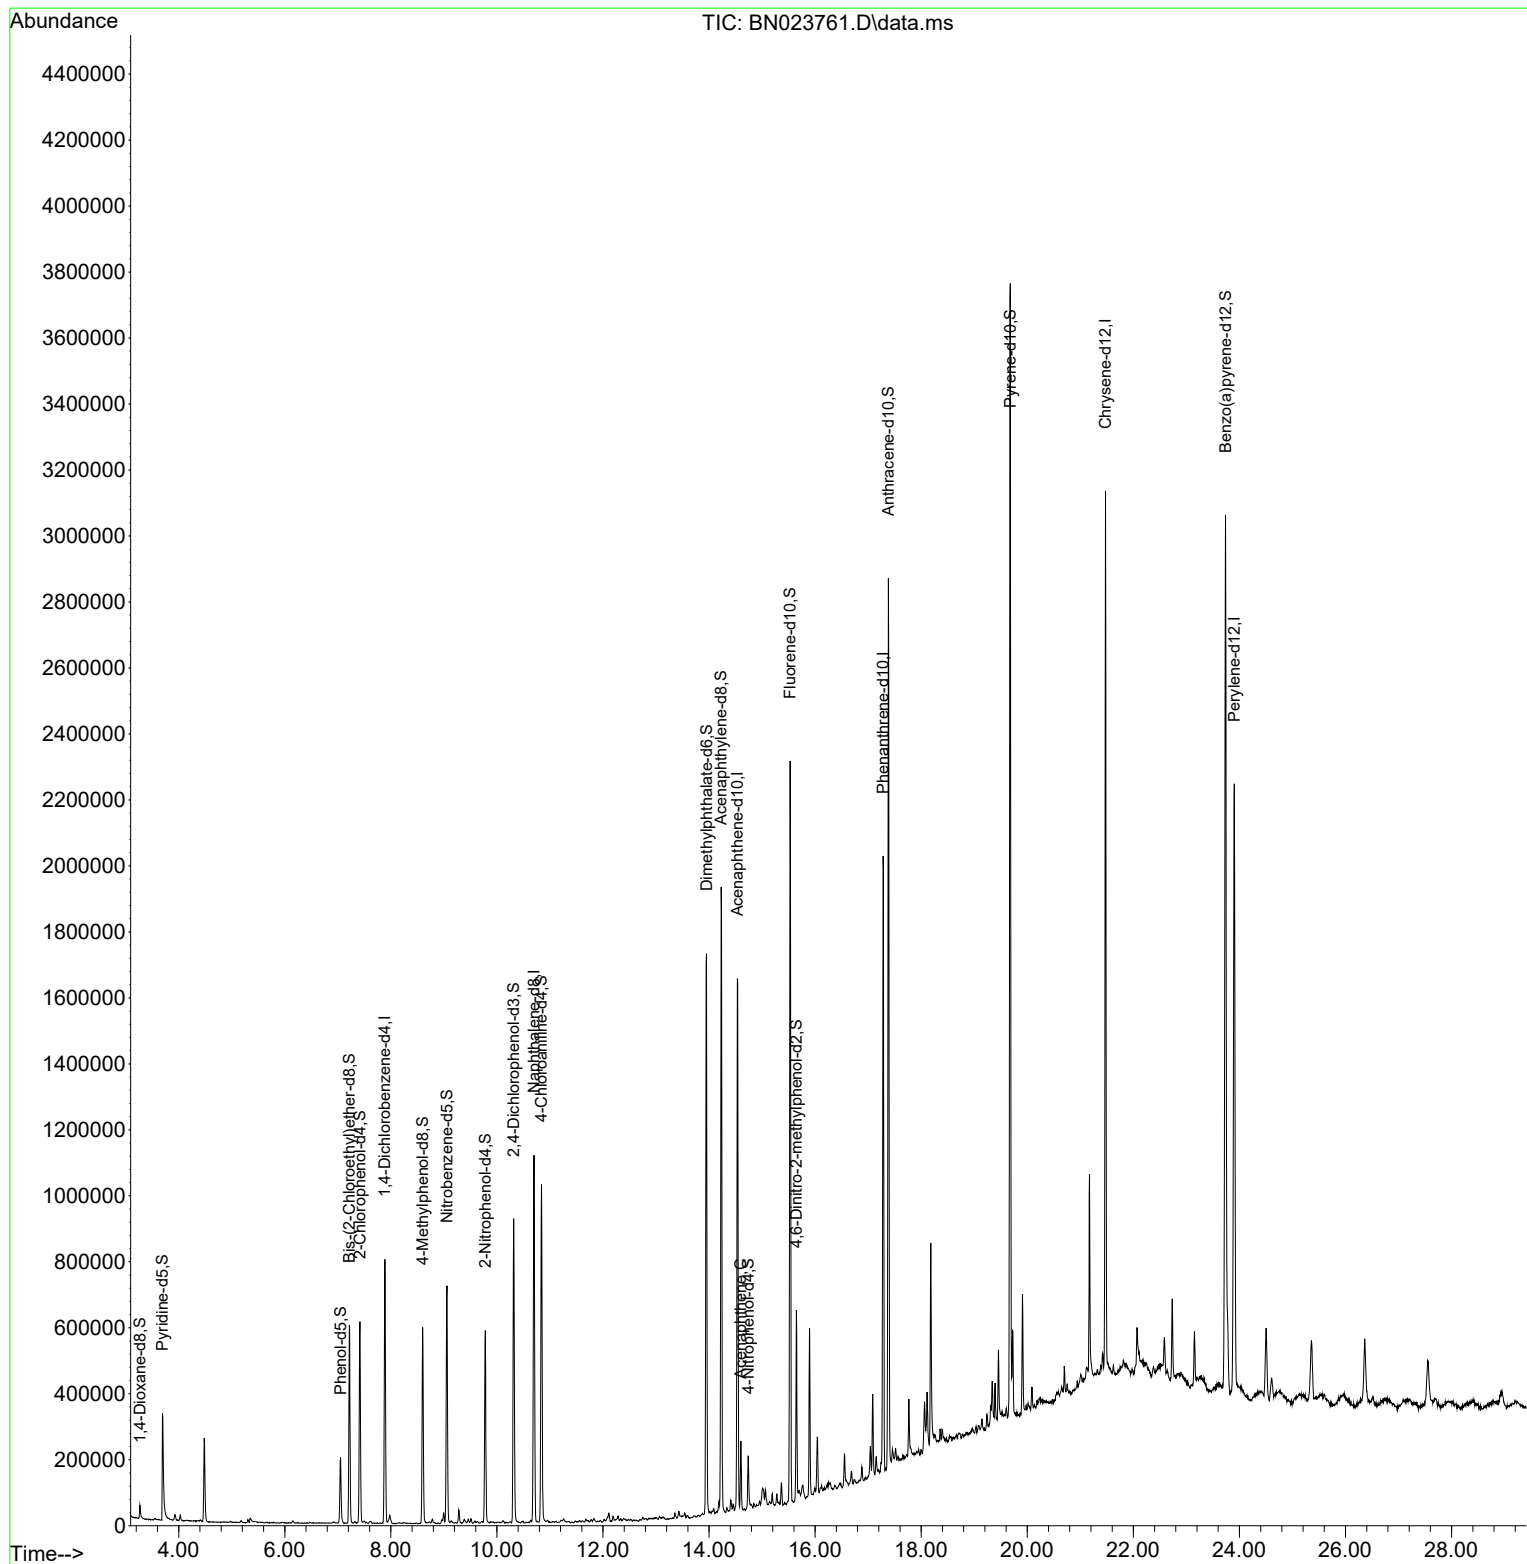

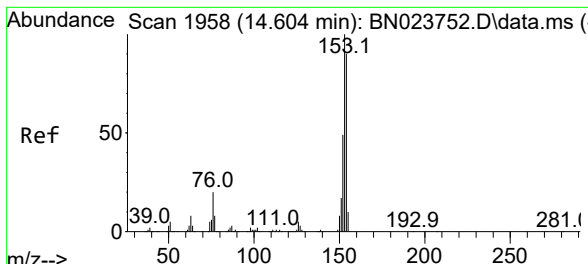

#52
 Acenaphthene
 Concen: 2.284 ng/ul
 RT: 14.598 min Scan# 1957
 Delta R.T. -0.006 min
 Lab File: BN023761.D
 Acq: 23 Jan 2023 20:34

Instrument :
 BNA_N
 ClientSampleId :
 EX9F7

Tgt Ion:	153	Resp:	76160
Ion Ratio	Lower	Upper	
153	100		
152	46.8	38.5	57.7
154	92.0	71.5	107.3

