

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023764.D
 Acq On : 23 Jan 2023 22:25
 Operator : CG/JU
 Sample : 01216-01DL2 50X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH206DL2

Quant Time: Jan 24 00:02:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	175502	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	755589	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	490111	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	1047798	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	1056286	20.000	ng/ul	-0.01
88) Perylene-d12	23.898	264	1065714	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.052	99	1564	0.101	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	6053	0.634	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	4853	0.407	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	3065	0.247	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	3281	0.576	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.775	143	2854	0.473	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.316	165	5394	0.469	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.846	131	10516m	0.581	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	23367	0.641	ng/ul	-0.01
49) Acenaphthylene-d8	14.228	160	22504	0.557	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.528	176	20471	0.657	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.381	188	30456	0.650	ng/ul	0.00
81) Pyrene-d10	19.675	212	39317	0.651	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	32082	0.609	ng/ul	-0.02
Target Compounds						
					Qvalue	
30) Naphthalene	10.751	128	3768977	92.790	ng/ul	100
36) 2-Methylnaphthalene	12.357	142	114841	4.241	ng/ul	100
37) 1-Methylnaphthalene	12.581	142	77874	2.815	ng/ul	99
77) Carbazole	17.686	167	56703	1.118	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023764.D
Acq On : 23 Jan 2023 22:25
Operator : CG/JU
Sample : 01216-01DL2 50X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BH206DL2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023

Quant Time: Jan 24 00:02:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

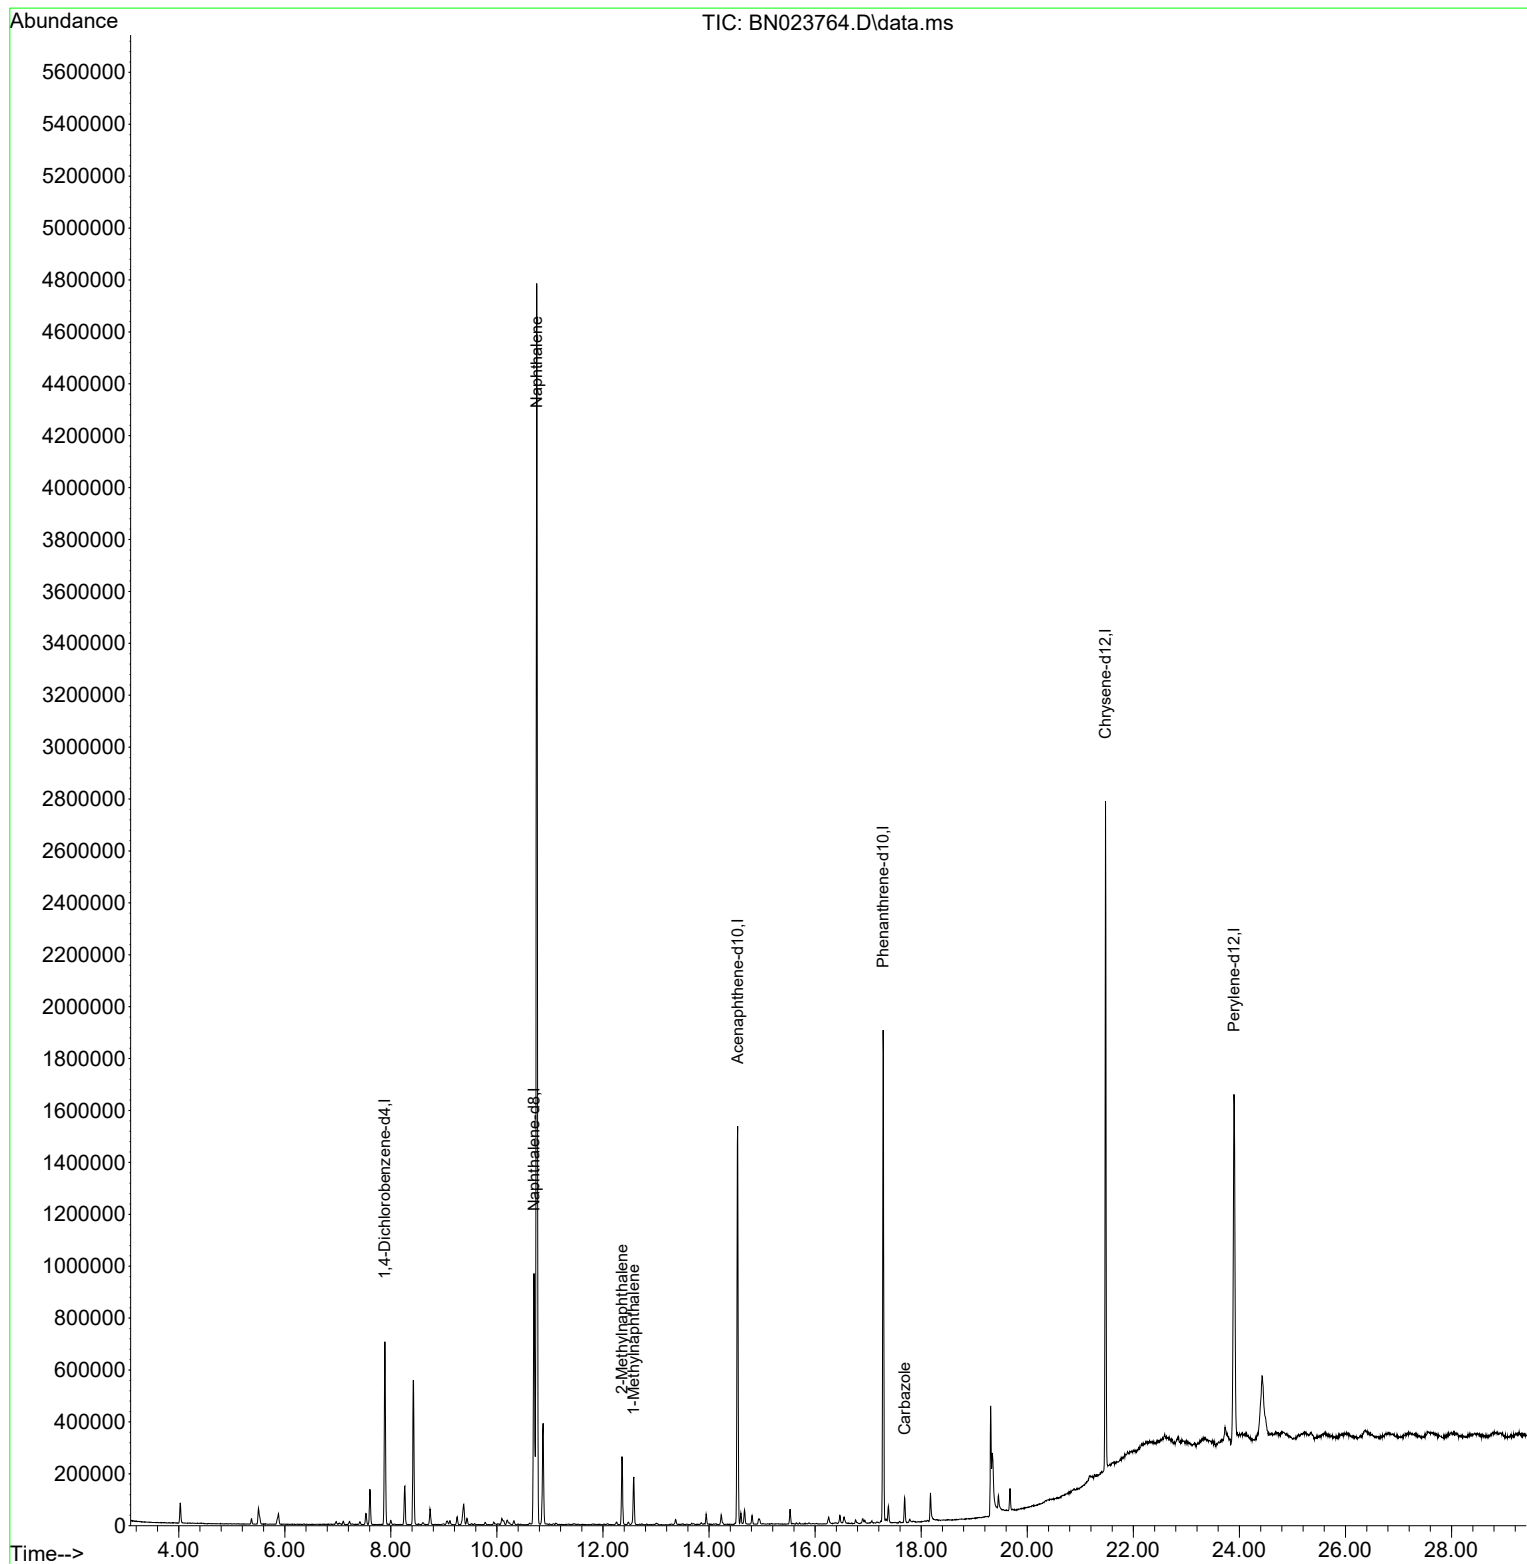

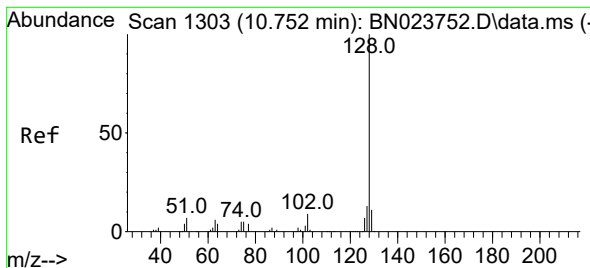

#30

Naphthalene

Concen: 92.790 ng/ul

RT: 10.751 min Scan# 11

Delta R.T. -0.006 min

Lab File: BN023764.D

Acq: 23 Jan 2023 22:25

Instrument :

BNA_N

ClientSampleId :

BH206DL2

Tgt Ion:128 Resp: 376897

Ion Ratio Lower Upper

128 100





129 11.1 9.1 13.7

127 13.6 10.8 16.2

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023

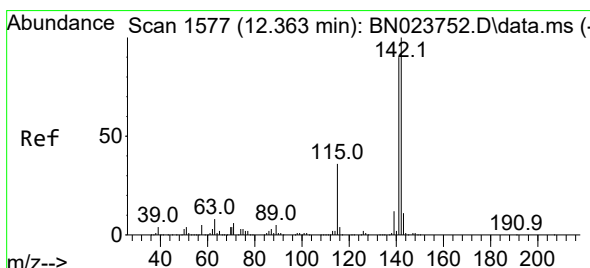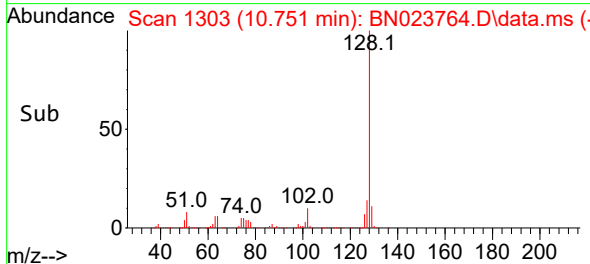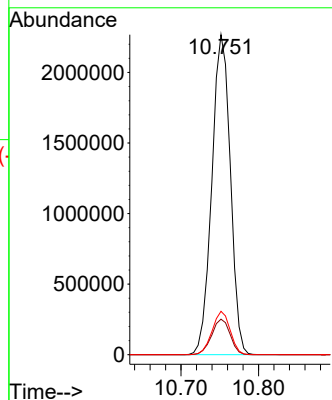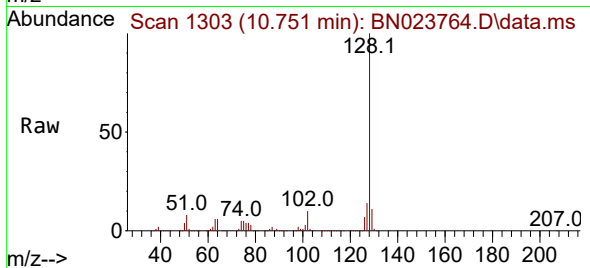

#36

2-Methylnaphthalene

Concen: 4.241 ng/ul

RT: 12.357 min Scan# 1576

Delta R.T. -0.006 min

Lab File: BN023764.D




Acq: 23 Jan 2023 22:25


Tgt Ion:142 Resp: 114841

Ion Ratio Lower Upper

142 100

141 91.7 73.6 110.4

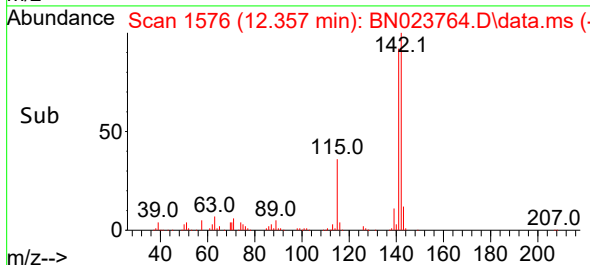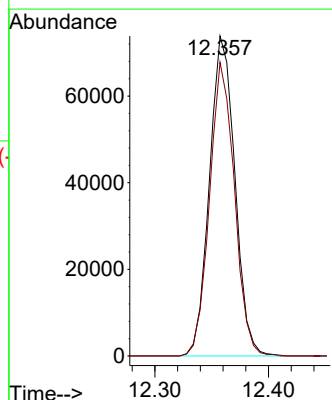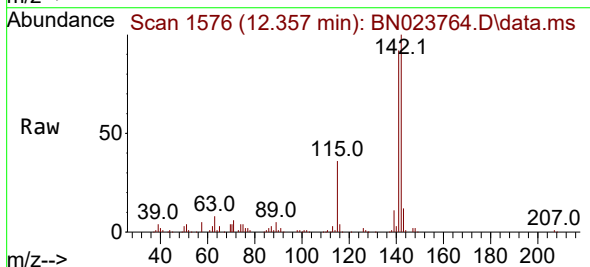

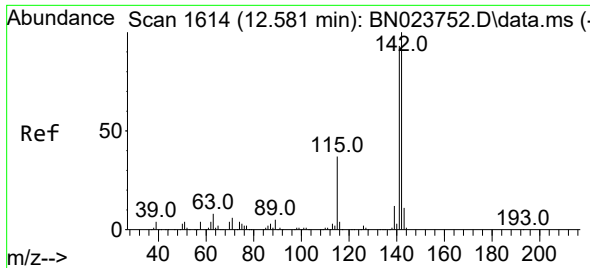

#37

1-Methylnaphthalene

Concen: 2.815 ng/ul

RT: 12.581 min Scan# 1

Delta R.T. -0.006 min

Lab File: BN023764.D

Acq: 23 Jan 2023 22:25

Instrument :

BNA_N

ClientSampleId :





BH206DL2

Tgt Ion:	142	Resp:	77874
Ion Ratio	Lower	Upper	
142	100		
141	91.6	73.8	110.6
116	3.8	3.0	4.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023

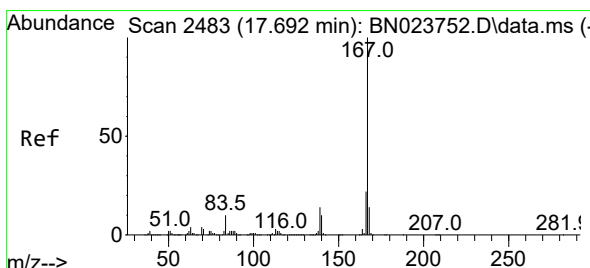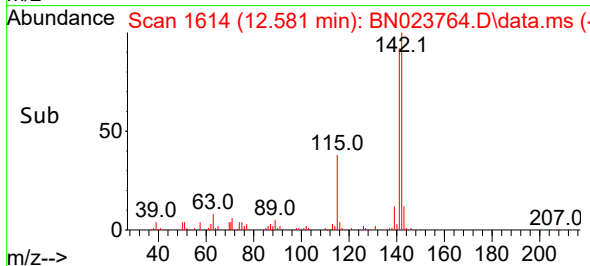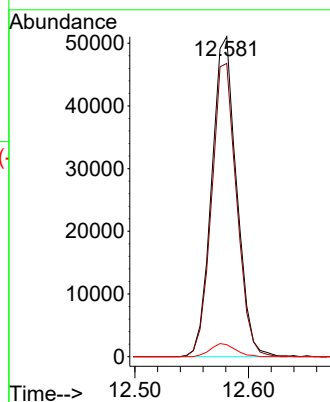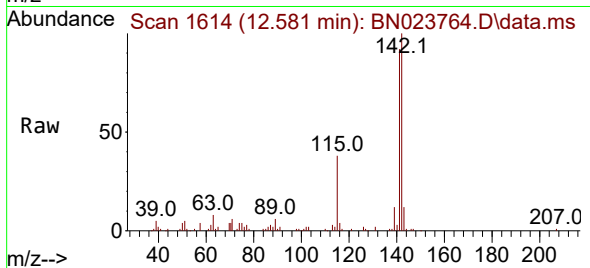

#77

Carbazole

Concen: 1.118 ng/ul

RT: 17.686 min Scan# 2482

Delta R.T. -0.006 min

Lab File: BN023764.D

Acq: 23 Jan 2023 22:25

Tgt Ion:	167	Resp:	56703
Ion Ratio	Lower	Upper	
167	100		
166	21.1	17.4	26.2
139	12.7	11.0	16.6

