

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023779.D
 Acq On : 24 Jan 2023 16:22
 Operator : CG/JU
 Sample : 01226-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9G5

Quant Time: Jan 24 23:58:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 24 23:52:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	231057	20.000	ng/u1	0.00
20) Naphthalene-d8	10.699	136	950716	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.534	164	558788	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.281	188	1021286	20.000	ng/u1	0.00
79) Chrysene-d12	21.474	240	927616	20.000	ng/u1	0.00
88) Perylene-d12	23.898	264	871913	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	20816	3.877	ng/uL	0.00
4) Pyridine-d5	3.699	84	133023	8.257	ng/u1	0.00
7) Phenol-d5	7.052	99	129454	6.322	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	312879	24.906	ng/u1	0.00
11) 2-Chlorophenol-d4	7.416	132	317685	20.256	ng/u1	0.00
15) 4-Methylphenol-d8	8.599	113	250386	15.319	ng/u1	0.00
21) Nitrobenzene-d5	9.057	128	204794	28.566	ng/u1	0.00
24) 2-Nitrophenol-d4	9.781	143	213015	28.068	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	380252	26.268	ng/u1	0.00
31) 4-Chloroaniline-d4	10.840	131	485016	21.301	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1347965	32.428	ng/u1	0.00
49) Acenaphthylene-d8	14.228	160	1426400	30.970	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	41710	4.929	ng/u1	0.00
60) Fluorene-d10	15.528	176	949531	26.733	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	171674	27.865	ng/u1	0.00
73) Anthracene-d10	17.381	188	1481938	32.427	ng/u1	0.00
81) Pyrene-d10	19.675	212	1837088	34.628	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.739	264	1378580	31.972	ng/u1	0.00
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.386	149	57445	1.525	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023779.D
Acq On : 24 Jan 2023 16:22
Operator : CG/JU
Sample : 01226-11
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9G5

Quant Time: Jan 24 23:58:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 24 23:52:16 2023
Response via : Initial Calibration

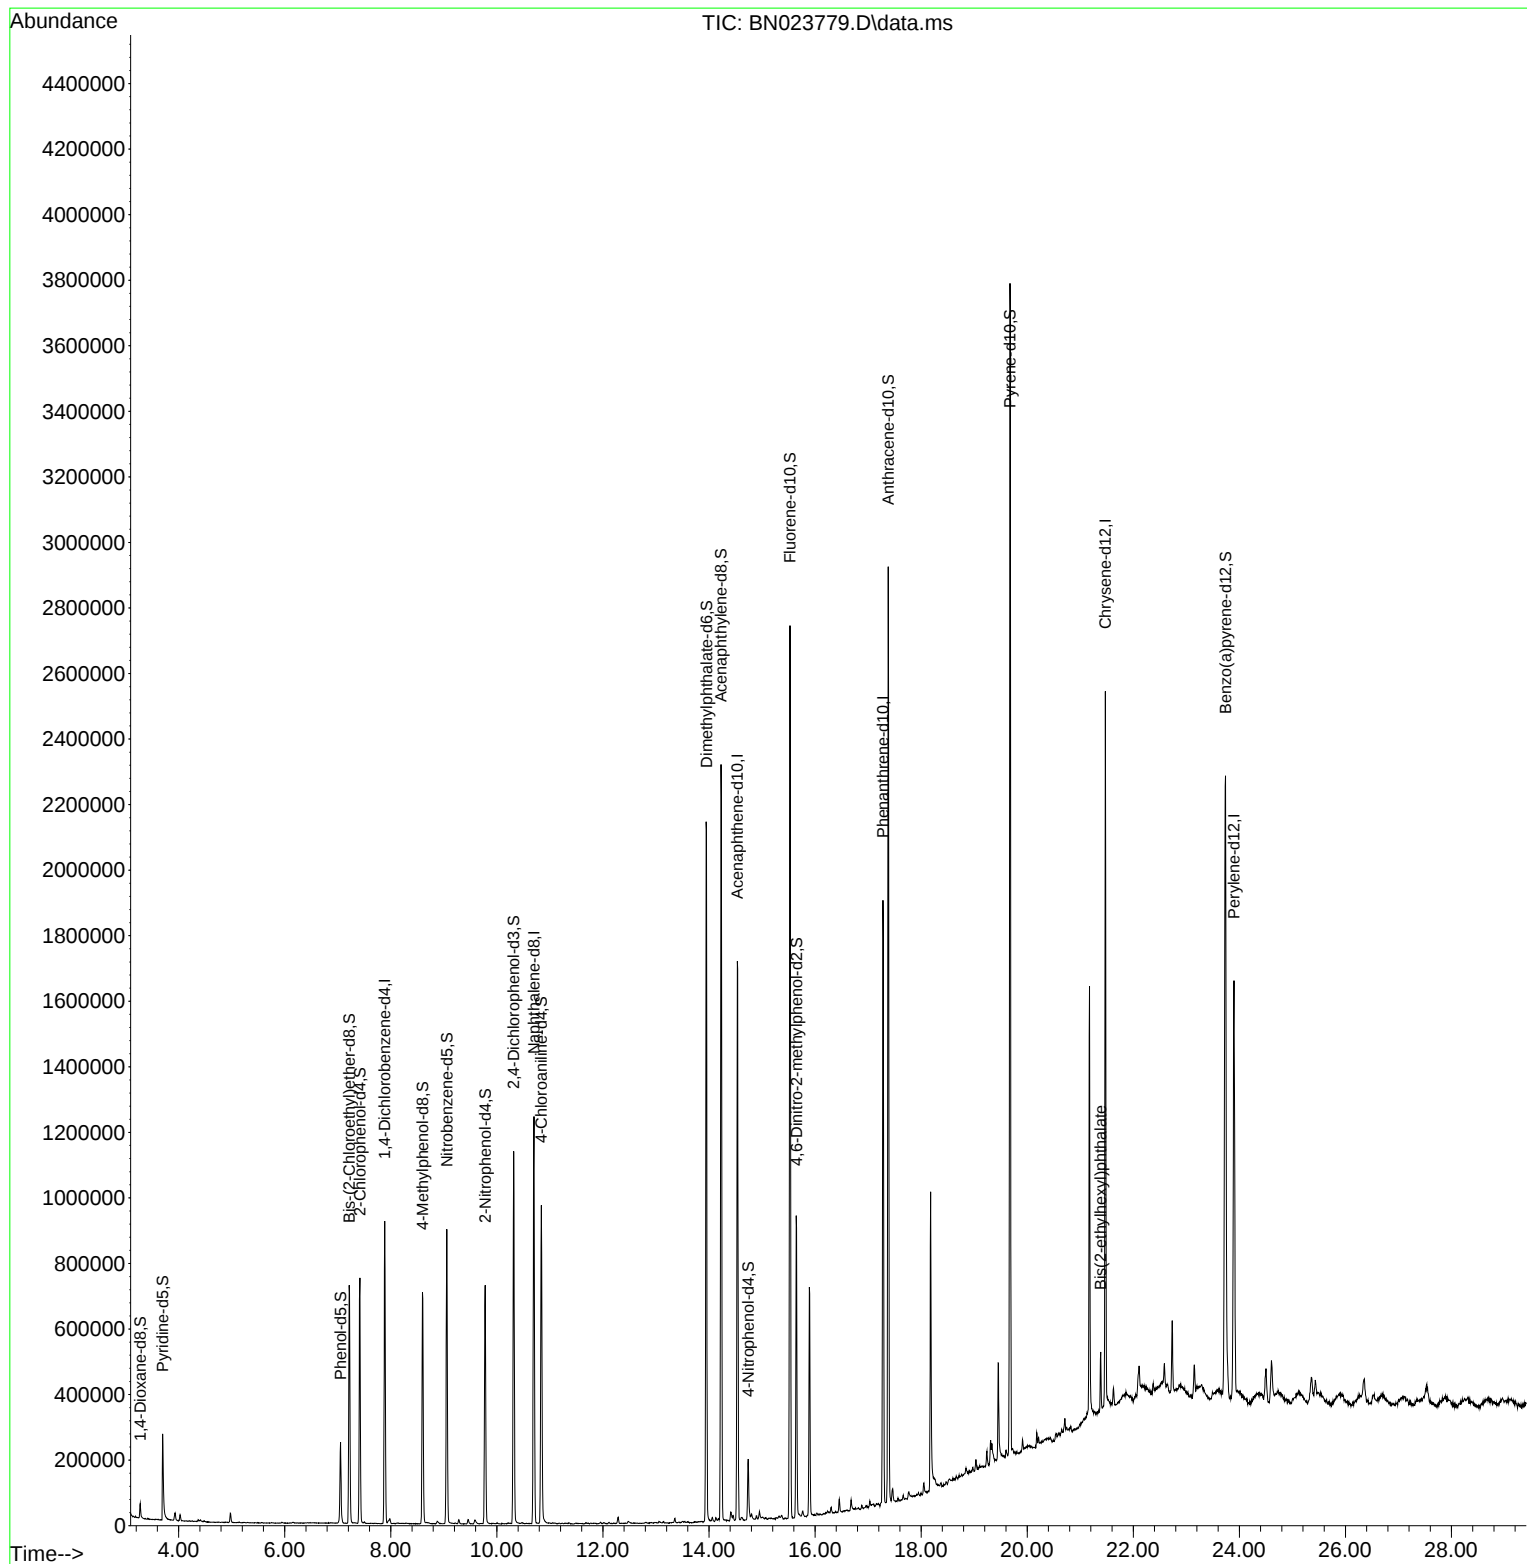

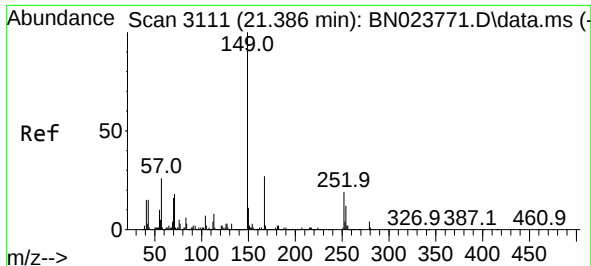

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.525 ng/ul
 RT: 21.386 min Scan# 3111
 Delta R.T. -0.000 min
 Lab File: BN023779.D
 Acq: 24 Jan 2023 16:22

Instrument :
 BNA_N
 ClientSampleId :
 EX9G5

Tgt Ion:149 Resp: 57445
 Ion Ratio Lower Upper
 149 100
 167 26.8 22.0 33.0
 279 4.4 3.4 5.2

