

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023748.D
 Acq On : 23 Jan 2023 12:19
 Operator : CG/JU
 Sample : PB150349BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	29	32	43	rVB	79898	114126	2.29%	0.197%
2	3.699	100	104	126	rBV	1027951	1555254	31.20%	2.679%
3	4.028	157	160	166	rVB	17825	25500	0.51%	0.044%
4	7.051	667	674	684	rBV	1226750	1893437	37.99%	3.262%
5	7.222	696	703	712	rBV	971431	1523713	30.57%	2.625%
6	7.416	729	736	751	rVB	1274892	1947504	39.07%	3.355%
7	7.887	809	816	824	rBV	945954	1420944	28.51%	2.448%
8	8.598	929	937	951	rBV	1428823	2248714	45.12%	3.874%
9	9.057	1007	1015	1026	rBV	1148255	1793000	35.97%	3.089%
10	9.781	1130	1138	1148	rBV	925672	1473396	29.56%	2.538%
11	10.316	1221	1229	1240	rBV	1399049	2224373	44.63%	3.832%
12	10.698	1286	1294	1302	rBV	1239297	1979403	39.71%	3.410%
13	10.839	1311	1318	1331	rBV	1421811	2335840	46.87%	4.024%
14	11.922	1487	1502	1503	rBV9	11751	28355	0.57%	0.049%
15	12.286	1559	1564	1571	rVB2	21482	36228	0.73%	0.062%
16	13.951	1836	1847	1861	rBV	2332394	3086515	61.93%	5.317%
17	14.233	1888	1895	1903	rBV	2610488	3665744	73.55%	6.315%
18	14.539	1940	1947	1957	rVB	1702609	2404471	48.24%	4.142%
19	14.733	1974	1980	1998	rBV	1002513	1438199	28.86%	2.477%
20	14.951	2013	2017	2022	rVB7	3666	6453	0.13%	0.011%
21	15.533	2107	2116	2128	rBV	3086297	4445559	89.19%	7.658%
22	15.651	2130	2136	2152	rVV	822232	1095167	21.97%	1.887%
23	15.769	2152	2156	2163	rVB	16266	23629	0.47%	0.041%
24	17.286	2407	2414	2421	rBV	1945815	2672017	53.61%	4.603%
25	17.386	2424	2431	2452	rVV	3337108	4589375	92.08%	7.906%
26	17.663	2474	2478	2483	rBV6	3020	5491	0.11%	0.009%
27	17.821	2501	2505	2509	rVB5	3427	6175	0.12%	0.011%
28	19.245	2742	2747	2751	rBV2	36084	51524	1.03%	0.089%
29	19.310	2754	2758	2764	rVV	33271	46182	0.93%	0.080%
30	19.680	2815	2821	2827	rBV	3817947	4984185	100.00%	8.586%
31	21.480	3122	3127	3133	rBV	1941958	2453024	49.22%	4.226%
32	23.751	3506	3513	3528	rVB2	1935143	4239115	85.05%	7.302%
33	23.909	3534	3540	3547	rBV2	1314127	2238514	44.91%	3.856%




Sum of corrected areas: 58051126

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023748.D
Acq On : 23 Jan 2023 12:19
Operator : CG/JU
Sample : PB150349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

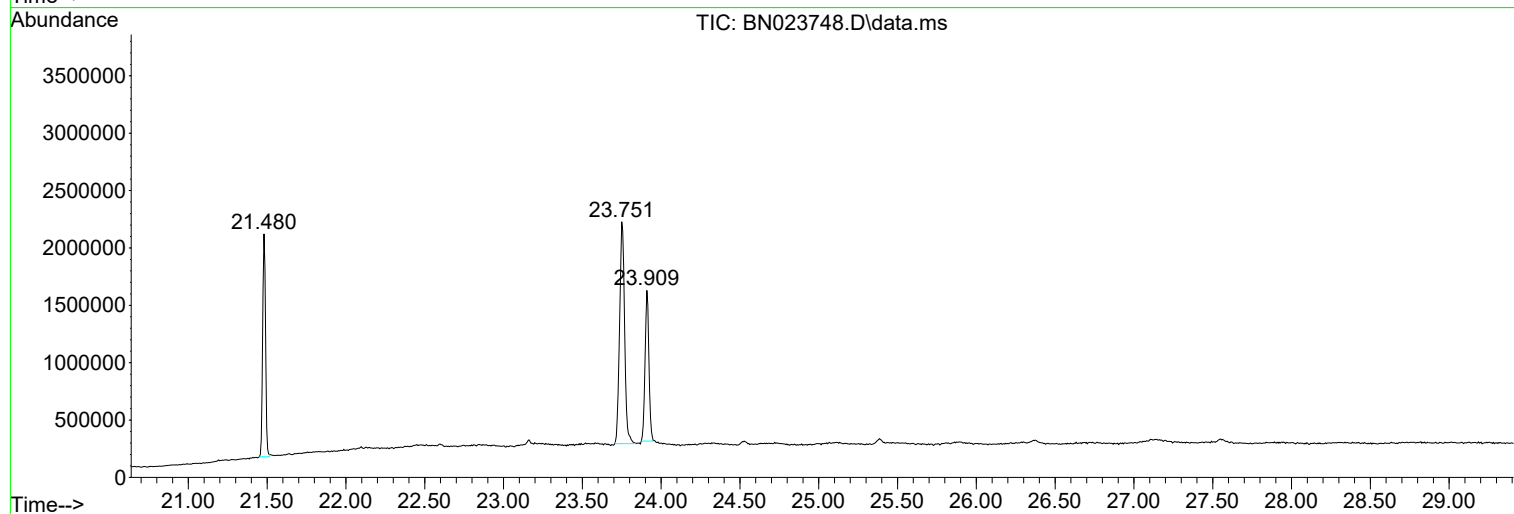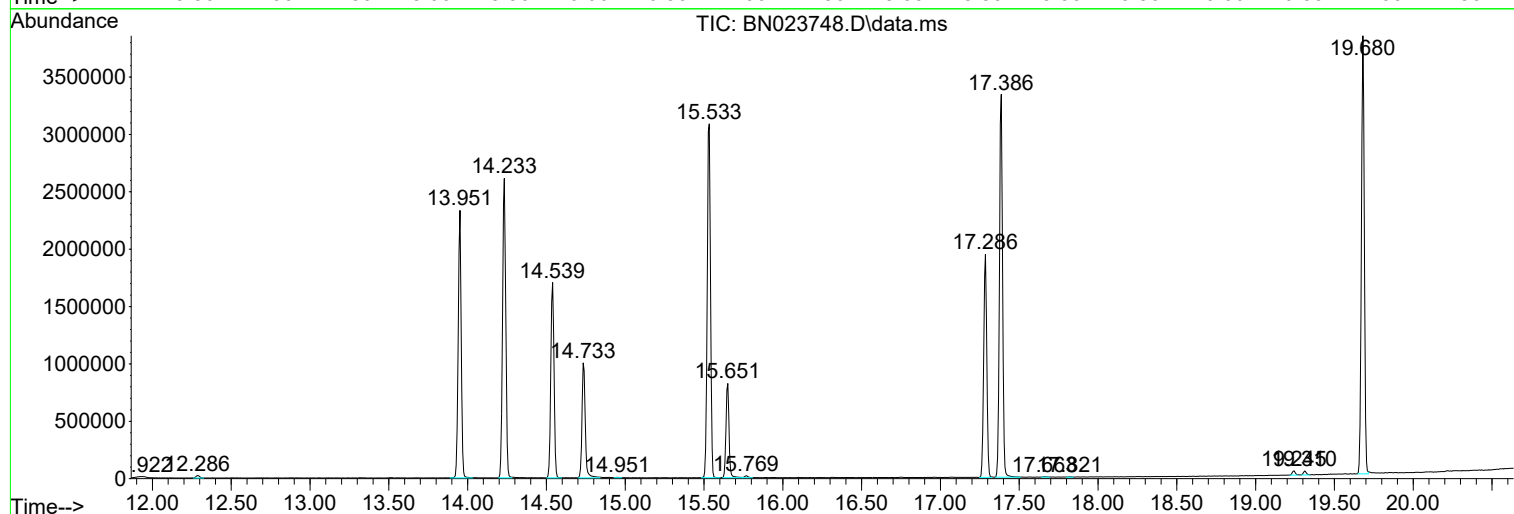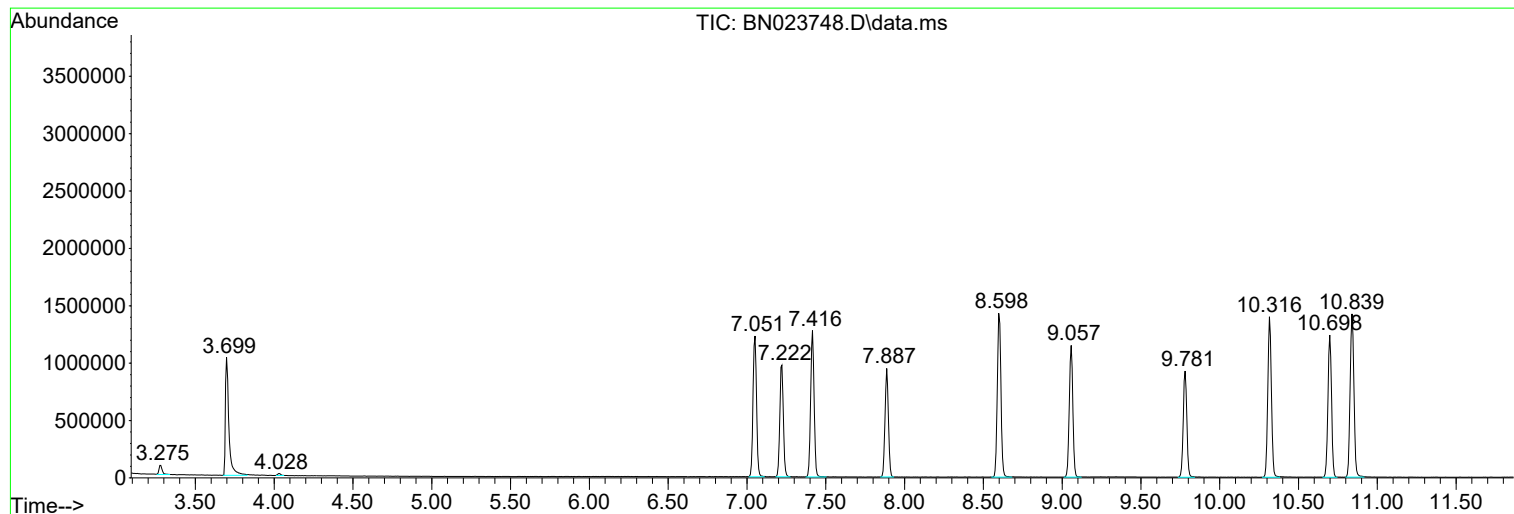

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023748.D
Acq On : 23 Jan 2023 12:19
Operator : CG/JU
Sample : PB150349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023748.D
Acq On : 23 Jan 2023 12:19
Operator : CG/JU
Sample : PB150349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc