

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023753.D
 Acq On : 23 Jan 2023 15:39
 Operator : CG/JU
 Sample : PB150401BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK401

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rBV	43261	63299	1.38%	0.151%
2	3.693	100	103	126	rBV	550265	915180	19.93%	2.190%
3	4.028	156	160	166	rVB2	11147	16849	0.37%	0.040%
4	7.052	667	674	686	rVB	736949	1135580	24.72%	2.718%
5	7.222	696	703	715	rVB	579750	917515	19.98%	2.196%
6	7.416	727	736	749	rBV	744392	1158959	25.23%	2.774%
7	7.887	808	816	825	rBV	626513	972303	21.17%	2.327%
8	8.599	931	937	951	rBV	885024	1346017	29.31%	3.221%
9	9.057	1006	1015	1023	rBV	686410	1069782	23.29%	2.560%
10	9.781	1130	1138	1152	rBV	538650	851991	18.55%	2.039%
11	10.316	1222	1229	1240	rBV	838451	1327620	28.90%	3.177%
12	10.699	1286	1294	1304	rVB	882138	1392844	30.32%	3.333%
13	10.840	1311	1318	1333	rBV	888052	1431136	31.16%	3.425%
14	11.946	1500	1506	1513	rVB3	4591	9646	0.21%	0.023%
15	12.287	1559	1564	1572	rBV	12702	22826	0.50%	0.055%
16	13.951	1840	1847	1854	rBV	1393620	1942886	42.30%	4.650%
17	14.234	1888	1895	1910	rBV	1600324	2262194	49.25%	5.414%
18	14.540	1940	1947	1955	rBV	1198293	1758206	38.28%	4.208%
19	14.734	1972	1980	1998	rBV	682101	968537	21.09%	2.318%
20	15.528	2108	2115	2124	rBV	2038913	2853253	62.12%	6.828%
21	15.645	2130	2135	2152	rBV	521157	731352	15.92%	1.750%
22	15.769	2152	2156	2162	rVB3	9430	12626	0.27%	0.030%
23	17.286	2407	2414	2424	rBV	1515080	2113934	46.02%	5.059%
24	17.381	2424	2430	2452	rVV	2269184	3165039	68.91%	7.574%
25	19.239	2742	2746	2751	rBV2	22694	31142	0.68%	0.075%
26	19.310	2754	2758	2764	rVV2	21978	30755	0.67%	0.074%
27	19.675	2814	2820	2828	rBV	2532266	3504228	76.29%	8.386%
28	21.480	3122	3127	3135	rBV	2077171	2486925	54.14%	5.952%
29	23.745	3505	3512	3530	rVB2	2303453	4593118	100.00%	10.992%
30	23.910	3533	3540	3549	rVV2	1423083	2699853	58.78%	6.461%




Sum of corrected areas: 41785595

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023753.D
Acq On : 23 Jan 2023 15:39
Operator : CG/JU
Sample : PB150401BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK401

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

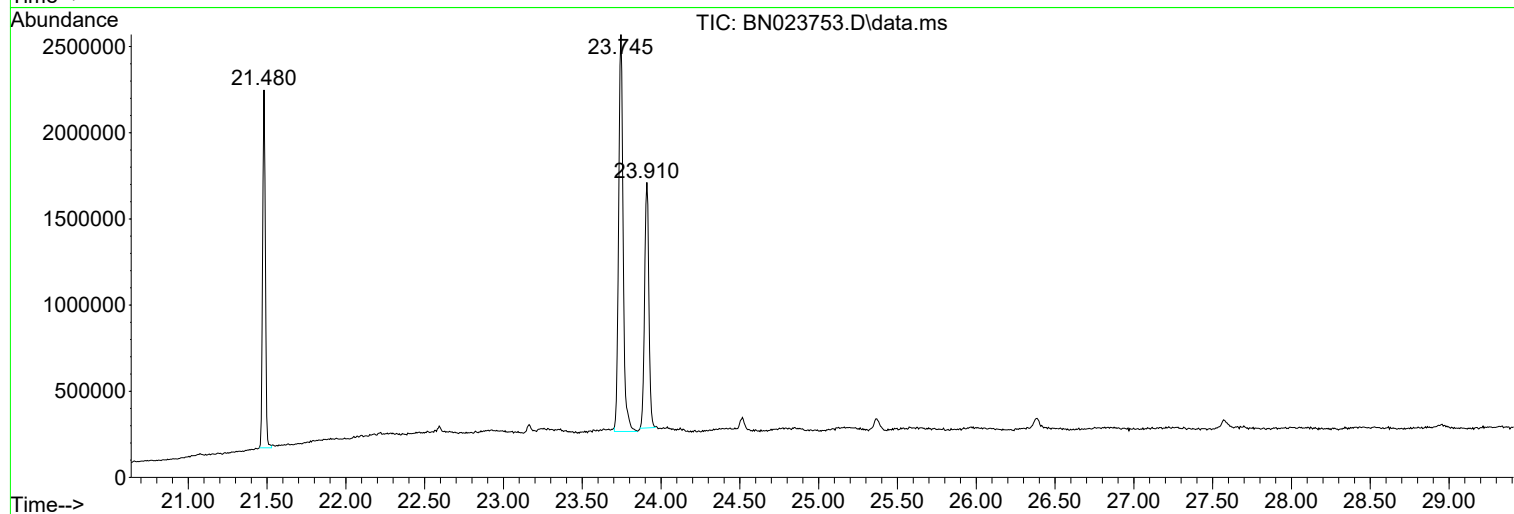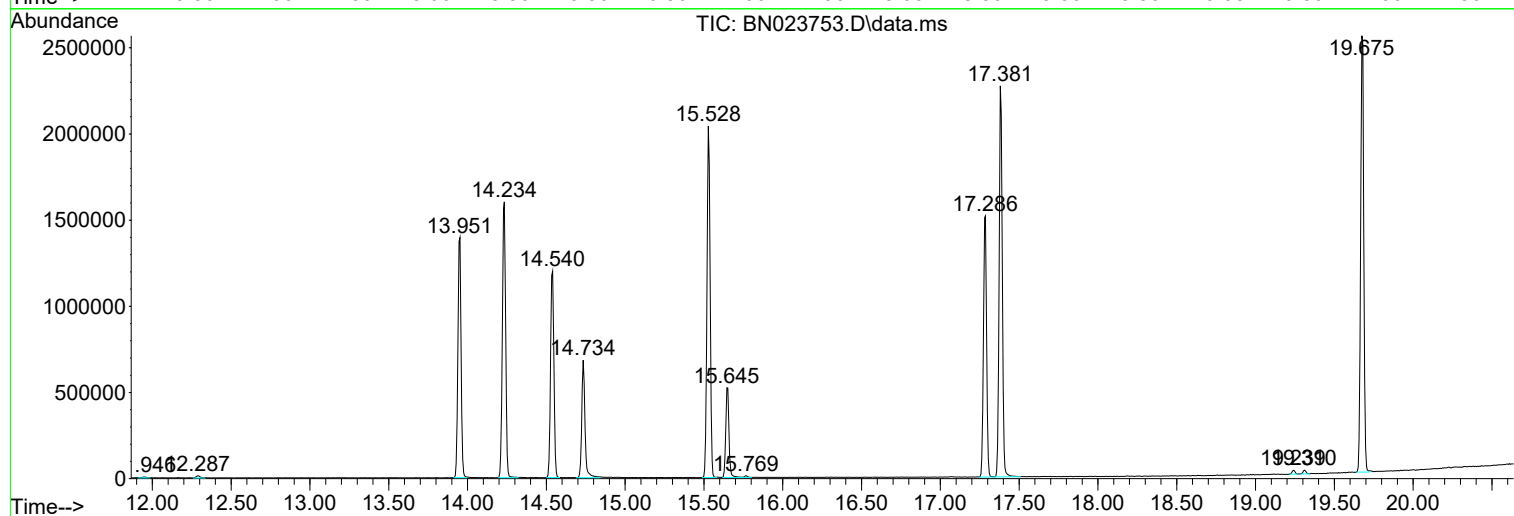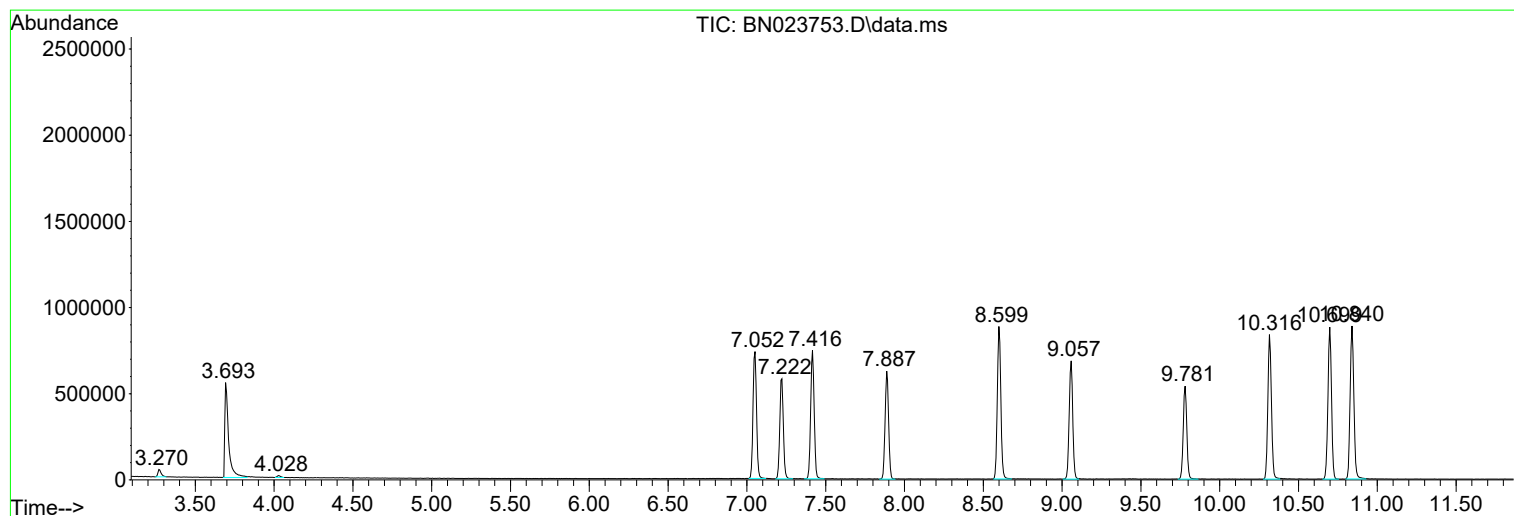

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023753.D
Acq On : 23 Jan 2023 15:39
Operator : CG/JU
Sample : PB150401BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK401

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023753.D
Acq On : 23 Jan 2023 15:39
Operator : CG/JU
Sample : PB150401BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK401

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc