

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023758.D
 Acq On : 23 Jan 2023 18:44
 Operator : CG/JU
 Sample : 01226-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9F4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	37	rVB	36354	47379	0.80%	0.091%
2	3.934	140	144	150	rVB	14892	22571	0.38%	0.043%
3	4.028	157	160	167	rVB	17614	26638	0.45%	0.051%
4	4.664	263	268	277	rBV	28945	46543	0.79%	0.090%
5	4.981	318	322	326	rVB3	5036	6712	0.11%	0.013%
6	6.299	541	546	550	rBV4	7385	11274	0.19%	0.022%
7	7.052	667	674	687	rVB	207808	317465	5.38%	0.612%
8	7.216	696	702	715	rVB	715355	1134444	19.22%	2.185%
9	7.416	729	736	747	rBV	780837	1192117	20.20%	2.297%
10	7.599	763	767	774	rVB7	3614	6698	0.11%	0.013%
11	7.887	809	816	825	rBV	867236	1337969	22.67%	2.578%
12	8.599	927	937	947	rBV	586332	912543	15.46%	1.758%
13	8.781	964	968	974	rVB2	9747	14930	0.25%	0.029%
14	9.058	1007	1015	1026	rBV	920111	1443903	24.47%	2.782%
15	9.510	1087	1092	1099	rVB2	12036	19284	0.33%	0.037%
16	9.781	1130	1138	1156	rBV	751372	1203076	20.39%	2.318%
17	10.316	1222	1229	1246	rBV	1078824	1716473	29.09%	3.307%
18	10.699	1286	1294	1307	rVB	1197266	1941392	32.90%	3.740%
19	10.840	1312	1318	1330	rVV	138061	239890	4.07%	0.462%
20	11.046	1349	1353	1357	rBV7	5472	8735	0.15%	0.017%
21	11.352	1400	1405	1409	rBV5	5262	8047	0.14%	0.016%
22	12.287	1559	1564	1571	rVB2	19680	29385	0.50%	0.057%
23	13.951	1840	1847	1857	rBV	1965031	2687375	45.54%	5.177%
24	14.234	1887	1895	1904	rBV	2179352	3107279	52.66%	5.986%
25	14.540	1940	1947	1956	rVB	1589072	2300841	38.99%	4.433%
26	14.734	1974	1980	1993	rBV	167506	271381	4.60%	0.523%
27	15.528	2109	2115	2123	rBV	2740765	3767435	63.84%	7.258%
28	15.645	2127	2135	2151	rBV	972120	1328240	22.51%	2.559%
29	15.763	2152	2155	2162	rVB2	11863	19130	0.32%	0.037%
30	16.963	2355	2359	2363	rBV6	4977	6897	0.12%	0.013%
31	17.069	2373	2377	2383	rVB3	4849	7834	0.13%	0.015%
32	17.287	2407	2414	2423	rBV	2192572	3059252	51.84%	5.894%
33	17.381	2424	2430	2448	rVV	3549040	4896041	82.97%	9.432%
34	17.951	2524	2527	2531	rVB6	5089	7092	0.12%	0.014%
35	18.175	2561	2565	2571	rBV2	34812	53934	0.91%	0.104%
36	19.239	2742	2746	2753	rVB2	47222	65912	1.12%	0.127%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023758.D
Acq On : 23 Jan 2023 18:44
Operator : CG/JU
Sample : 01226-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9F4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Title : SVOA CALIBRATION

37	19.310	2754	2758	2762	rBV2	53314	77112	1.31%	0.149%
38	19.451	2778	2782	2790	rBV	39331	66070	1.12%	0.127%
39	19.604	2805	2808	2812	rBV5	18733	22531	0.38%	0.043%
40	19.675	2814	2820	2831	rVV	4287503	5745173	97.36%	11.068%
41	21.475	3121	3126	3134	rBV	2814871	3380990	57.30%	6.513%
42	23.739	3503	3511	3526	rVB2	2751497	5900914	100.00%	11.368%
43	23.904	3532	3539	3551	rVB2	1764788	3449314	58.45%	6.645%




Sum of corrected areas: 51908215

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023758.D
Acq On : 23 Jan 2023 18:44
Operator : CG/JU
Sample : 01226-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9F4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

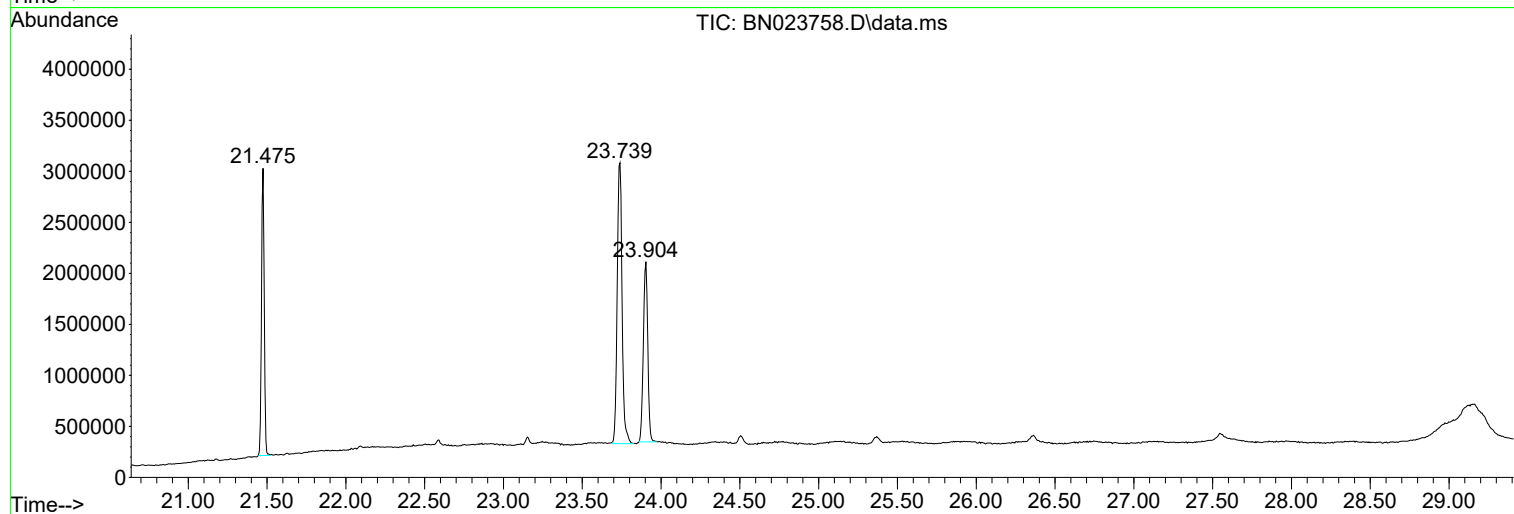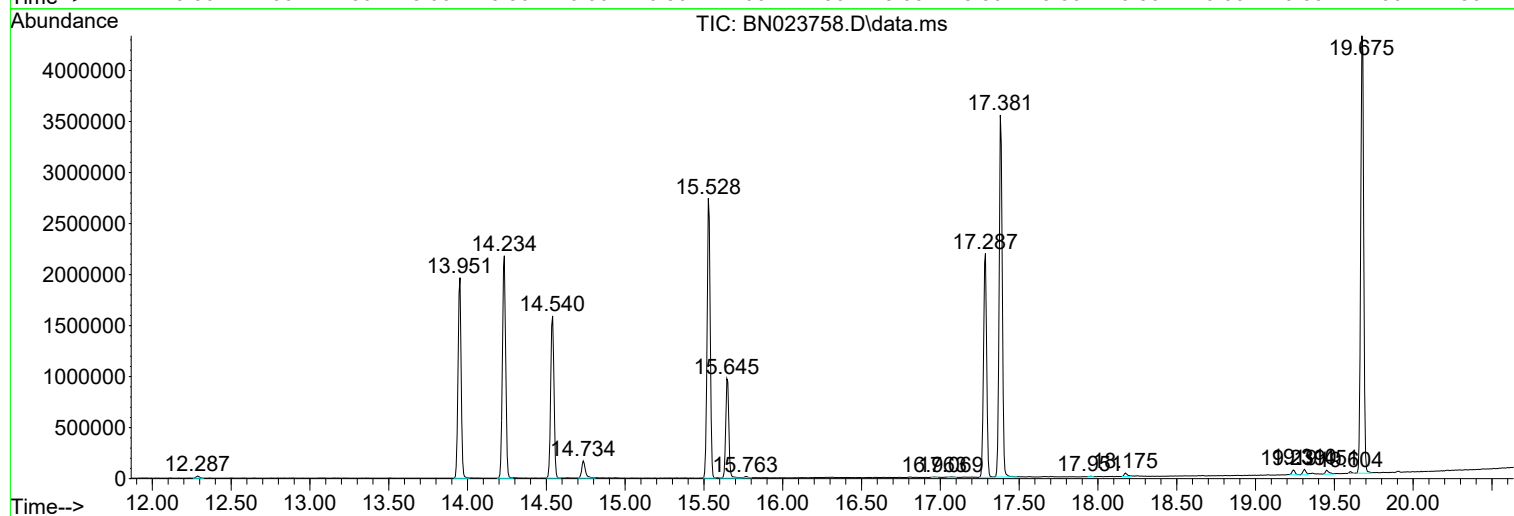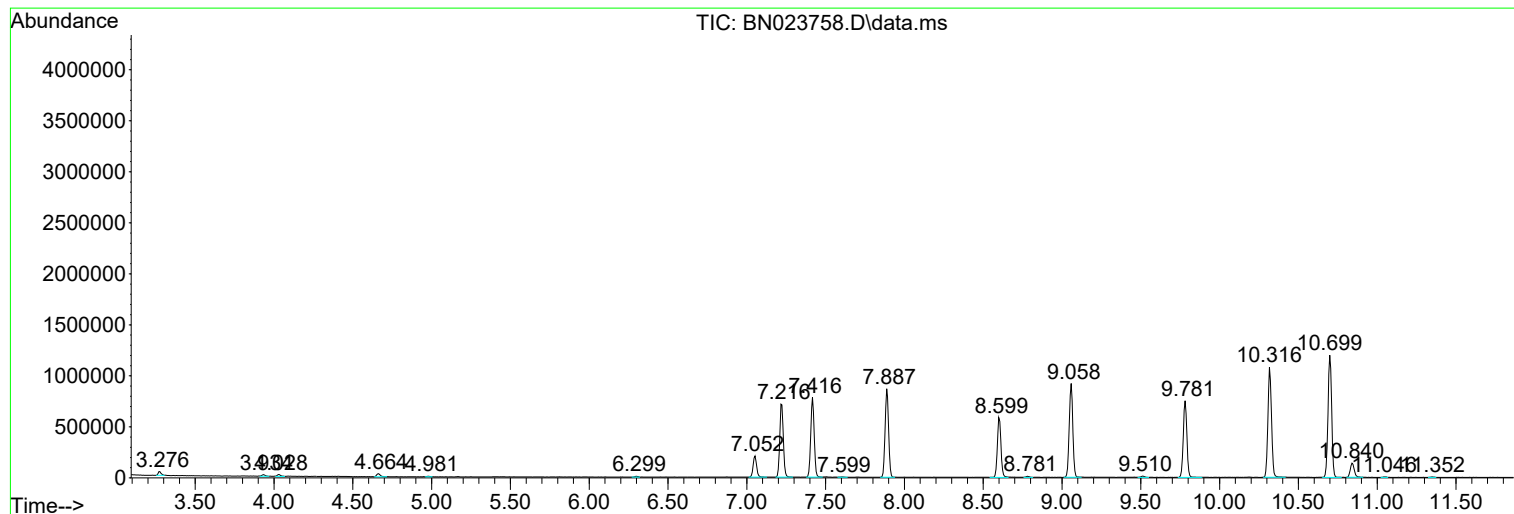

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023758.D
Acq On : 23 Jan 2023 18:44
Operator : CG/JU
Sample : 01226-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9F4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023758.D
Acq On : 23 Jan 2023 18:44
Operator : CG/JU
Sample : 01226-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9F4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc