

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023766.D
 Acq On : 23 Jan 2023 23:38
 Operator : CG/JU
 Sample : PB150404BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB	61209	82147	1.53%	0.158%
2	3.693	100	103	124	rBV	806958	1173471	21.90%	2.252%
3	4.028	156	160	166	rVB	16243	22127	0.41%	0.042%
4	7.052	667	674	686	rBV	1006597	1531955	28.59%	2.940%
5	7.216	696	702	717	rVB	780436	1210851	22.60%	2.324%
6	7.416	729	736	747	rBV	1031663	1562830	29.17%	3.000%
7	7.887	809	816	823	rBV	795380	1224084	22.85%	2.349%
8	8.599	930	937	949	rBV	1176907	1852156	34.57%	3.555%
9	9.057	1007	1015	1026	rBV	859706	1360074	25.38%	2.610%
10	9.781	1129	1138	1150	rBV	695795	1110357	20.72%	2.131%
11	10.316	1220	1229	1243	rBV	1023708	1642788	30.66%	3.153%
12	10.699	1286	1294	1304	rVB	912882	1503515	28.06%	2.886%
13	10.840	1310	1318	1332	rBV	1046383	1712883	31.97%	3.288%
14	12.287	1559	1564	1570	rVB	15535	24213	0.45%	0.046%
15	13.945	1840	1846	1862	rVB	1737031	2404783	44.88%	4.615%
16	14.228	1887	1894	1905	rBV2	2019199	2841377	53.03%	5.453%
17	14.534	1940	1946	1953	rBV	1365538	1988954	37.12%	3.817%
18	14.734	1973	1980	2001	rBV	888290	1291767	24.11%	2.479%
19	15.528	2108	2115	2124	rBV	2518826	3474520	64.85%	6.669%
20	15.645	2130	2135	2152	rBV	765609	1010634	18.86%	1.940%
21	15.763	2152	2155	2160	rVB	11950	15293	0.29%	0.029%
22	16.316	2244	2249	2252	rBV7	2880	5500	0.10%	0.011%
23	17.281	2407	2413	2424	rBV	1788928	2453957	45.80%	4.710%
24	17.381	2424	2430	2442	rBV	2752666	3848893	71.83%	7.387%
25	19.239	2742	2746	2752	rBV	43634	57697	1.08%	0.111%
26	19.310	2754	2758	2762	rVV	36405	47448	0.89%	0.091%
27	19.680	2814	2821	2831	rBV	3762163	5206450	97.17%	9.993%
28	21.474	3121	3126	3132	rBV2	2504321	3084851	57.57%	5.921%
29	23.733	3503	3510	3525	rVB2	2613884	5357996	100.00%	10.284%
30	23.898	3531	3538	3548	rBV2	1464321	2999057	55.97%	5.756%




Sum of corrected areas: 52102628

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023766.D
Acq On : 23 Jan 2023 23:38
Operator : CG/JU
Sample : PB150404BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

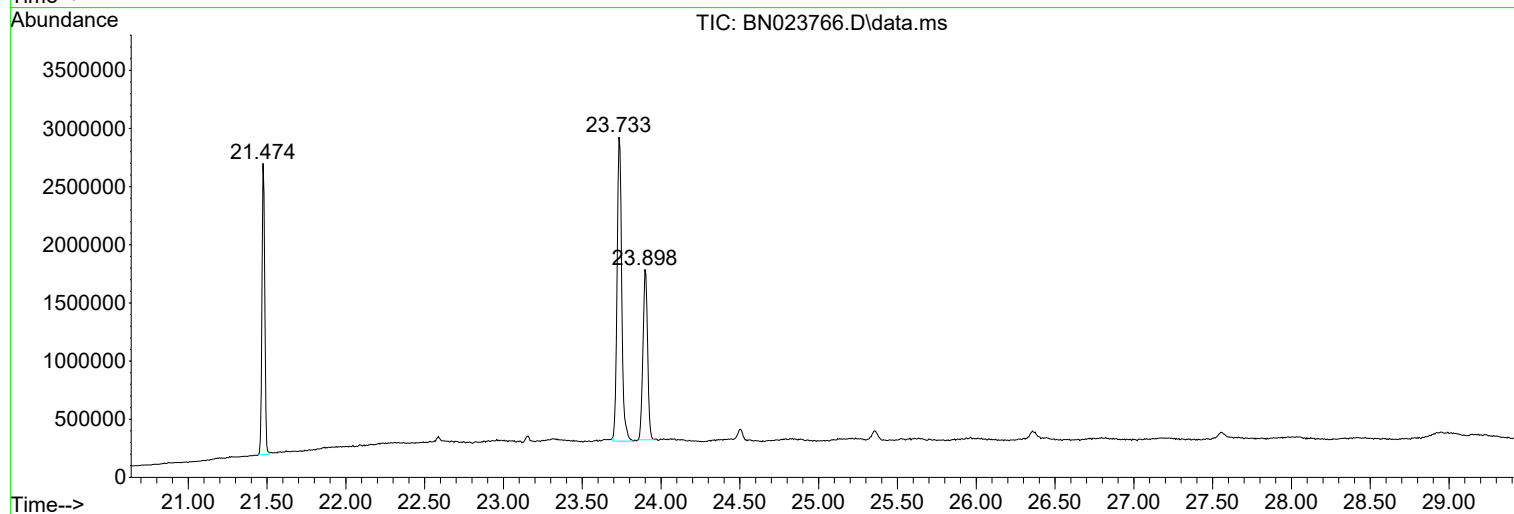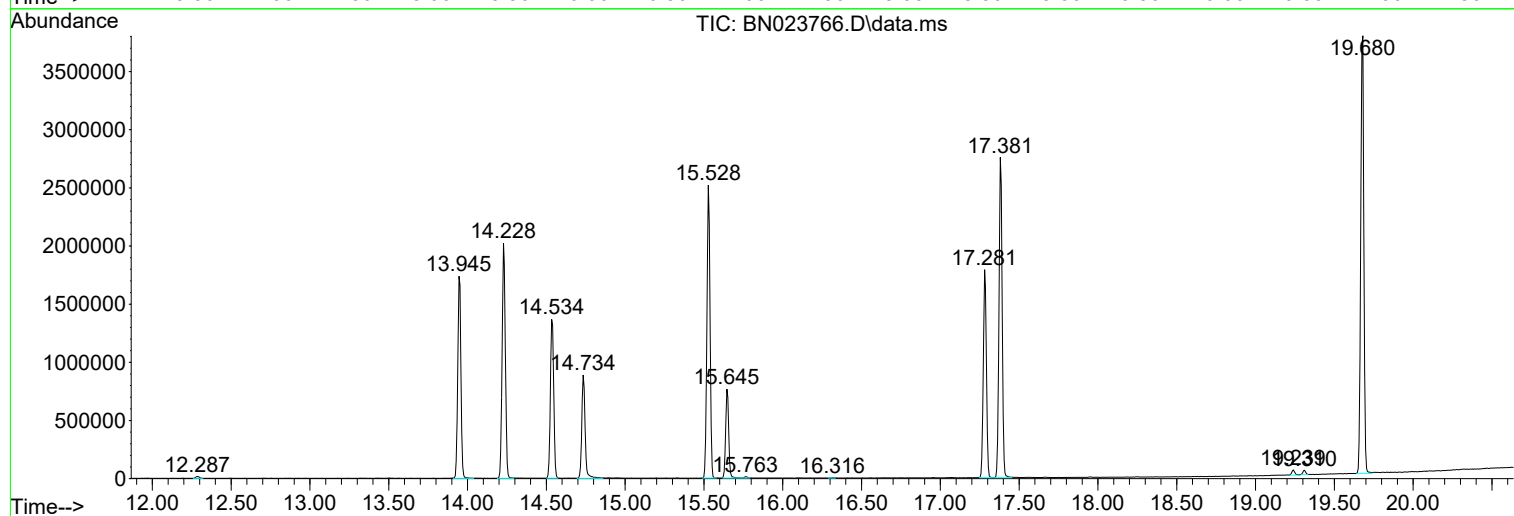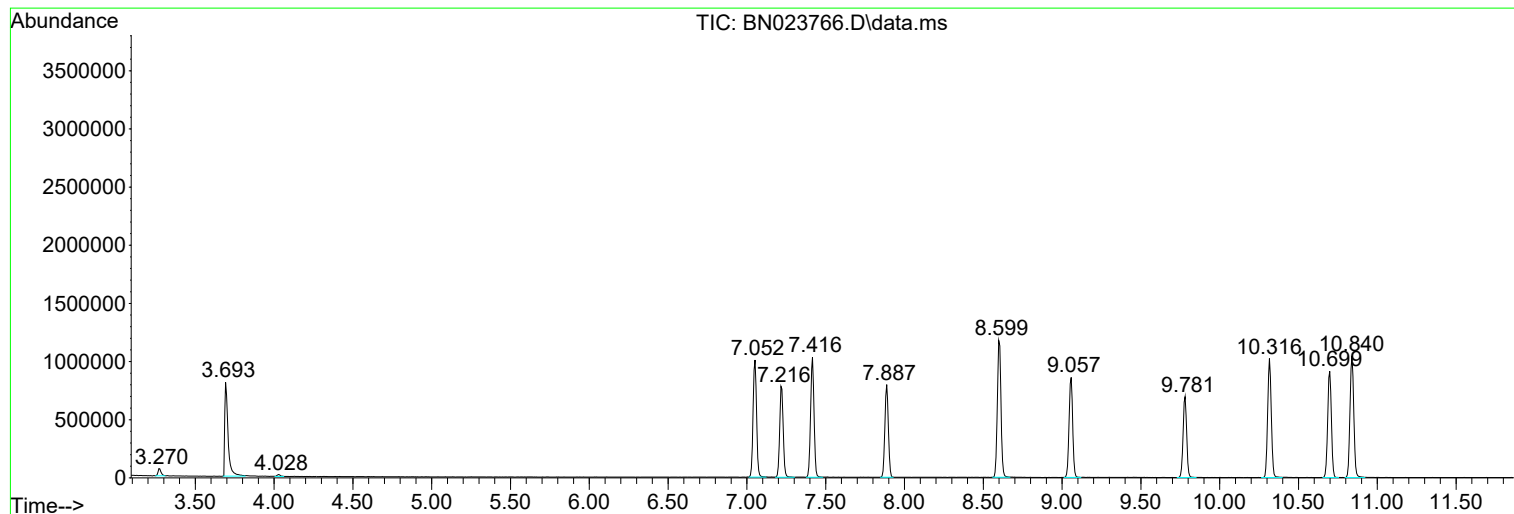

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023766.D
Acq On : 23 Jan 2023 23:38
Operator : CG/JU
Sample : PB150404BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023766.D
Acq On : 23 Jan 2023 23:38
Operator : CG/JU
Sample : PB150404BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc