

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023768.D
 Acq On : 24 Jan 2023 09:34
 Operator : CG/JU
 Sample : PB150407BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	41	rVB	72751	102447	2.73%	0.215%
2	3.693	99	103	127	rBV	921106	1334540	35.51%	2.804%
3	4.028	155	160	165	rVB	17679	26236	0.70%	0.055%
4	7.040	666	672	685	rBV	1043885	1606364	42.74%	3.376%
5	7.211	694	701	712	rVB	865807	1288601	34.28%	2.708%
6	7.405	727	734	747	rBV	1072500	1674479	44.55%	3.519%
7	7.881	808	815	822	rVB	855827	1311715	34.90%	2.756%
8	8.593	929	936	947	rBV	1209282	1866012	49.65%	3.921%
9	9.046	1006	1013	1025	rBV	926634	1491634	39.68%	3.135%
10	9.775	1130	1137	1151	rBV	769207	1241426	33.03%	2.609%
11	10.310	1220	1228	1238	rBV	1180080	1866216	49.65%	3.922%
12	10.693	1285	1293	1301	rBV	1101806	1755222	46.70%	3.688%
13	10.834	1309	1317	1328	rBV	1129069	1880573	50.03%	3.952%
14	12.281	1558	1563	1569	rVB	18164	27349	0.73%	0.057%
15	13.475	1747	1766	1767	rBV8	8257	28827	0.77%	0.061%
16	13.945	1840	1846	1857	rVB	1782231	2339628	62.25%	4.917%
17	14.228	1887	1894	1907	rVV	2088943	2903364	77.24%	6.101%
18	14.534	1940	1946	1954	rVB	1422488	2010308	53.48%	4.224%
19	14.734	1973	1980	1995	rBV	761646	1090355	29.01%	2.291%
20	14.945	2013	2016	2019	rVB5	3081	4075	0.11%	0.009%
21	15.263	2064	2070	2073	rBV8	3432	6933	0.18%	0.015%
22	15.416	2089	2096	2099	rBV5	12600	28734	0.76%	0.060%
23	15.463	2099	2104	2105	rVV4	15550	30273	0.81%	0.064%
24	15.528	2109	2115	2123	rVB	2448429	3404047	90.56%	7.153%
25	15.645	2129	2135	2149	rBV	661508	841953	22.40%	1.769%
26	15.763	2151	2155	2160	rVB2	10001	13644	0.36%	0.029%
27	16.345	2249	2254	2255	rBV5	4152	7035	0.19%	0.015%
28	16.557	2284	2290	2296	rBV4	6486	13826	0.37%	0.029%
29	16.734	2314	2320	2327	rBV2	25024	45586	1.21%	0.096%
30	17.069	2373	2377	2380	rBV3	3076	4452	0.12%	0.009%
31	17.110	2380	2384	2390	rVB3	7386	11933	0.32%	0.025%
32	17.186	2393	2397	2402	rVB7	4864	8193	0.22%	0.017%
33	17.281	2406	2413	2421	rBV	1599282	2159748	57.46%	4.539%
34	17.381	2423	2430	2443	rBV	2552921	3436830	91.44%	7.222%
35	17.669	2474	2479	2483	rVB3	9388	13617	0.36%	0.029%
36	17.816	2499	2504	2512	rVB	23842	36217	0.96%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023768.D
 Acq On : 24 Jan 2023 09:34
 Operator : CG/JU
 Sample : PB150407BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

37	17.945	2522	2526	2531	rVB6	7893	12108	0.32%	0.025%
38	18.175	2559	2565	2569	rBV9	7645	14037	0.37%	0.029%
39	18.639	2642	2644	2649	rVB3	5312	6206	0.17%	0.013%
40	18.704	2653	2655	2659	rVB4	4934	5359	0.14%	0.011%
41	18.763	2662	2665	2669	rVV3	17688	22543	0.60%	0.047%
42	19.239	2742	2746	2752	rBV3	28882	40407	1.08%	0.085%
43	19.310	2754	2758	2764	rBV	26349	40156	1.07%	0.084%
44	19.563	2797	2801	2806	rBV2	22823	33538	0.89%	0.070%
45	19.675	2814	2820	2827	rBV	2721297	3758701	100.00%	7.899%
46	20.263	2917	2920	2925	rBV2	20357	28814	0.77%	0.061%
47	21.475	3121	3126	3132	rBV	1602911	1962437	52.21%	4.124%
48	23.745	3505	3512	3523	rBV2	1829422	3642782	96.92%	7.655%
49	23.898	3531	3538	3546	rVB2	1099745	2107559	56.07%	4.429%




Sum of corrected areas: 47587039

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023768.D
Acq On : 24 Jan 2023 09:34
Operator : CG/JU
Sample : PB150407BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

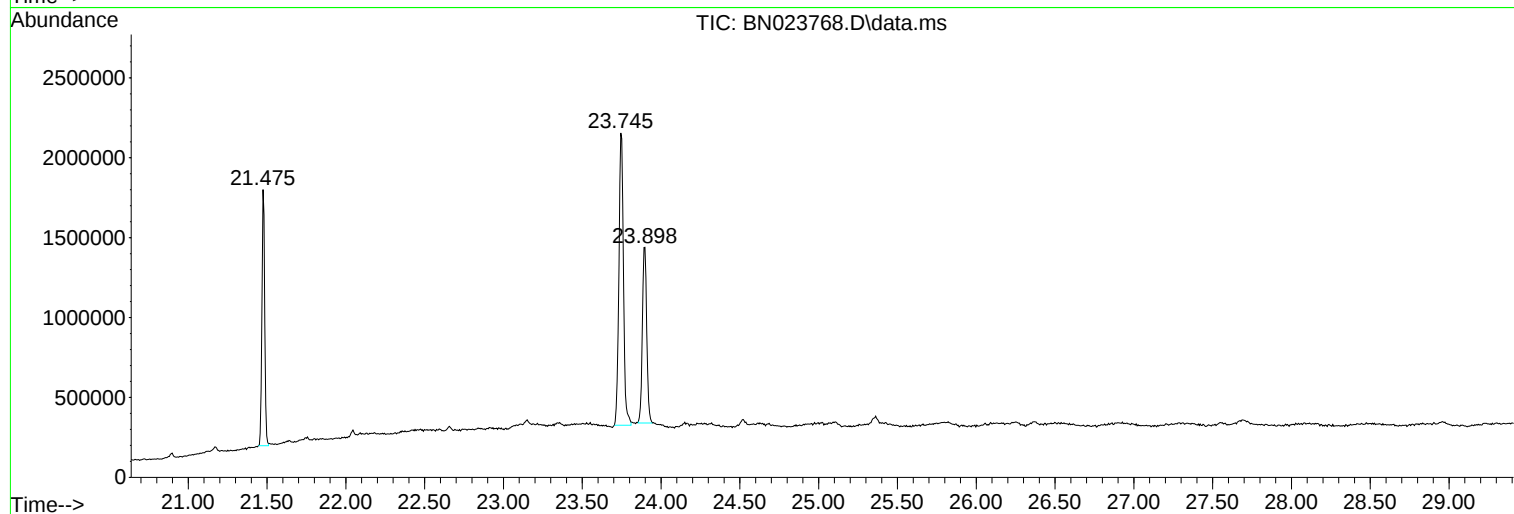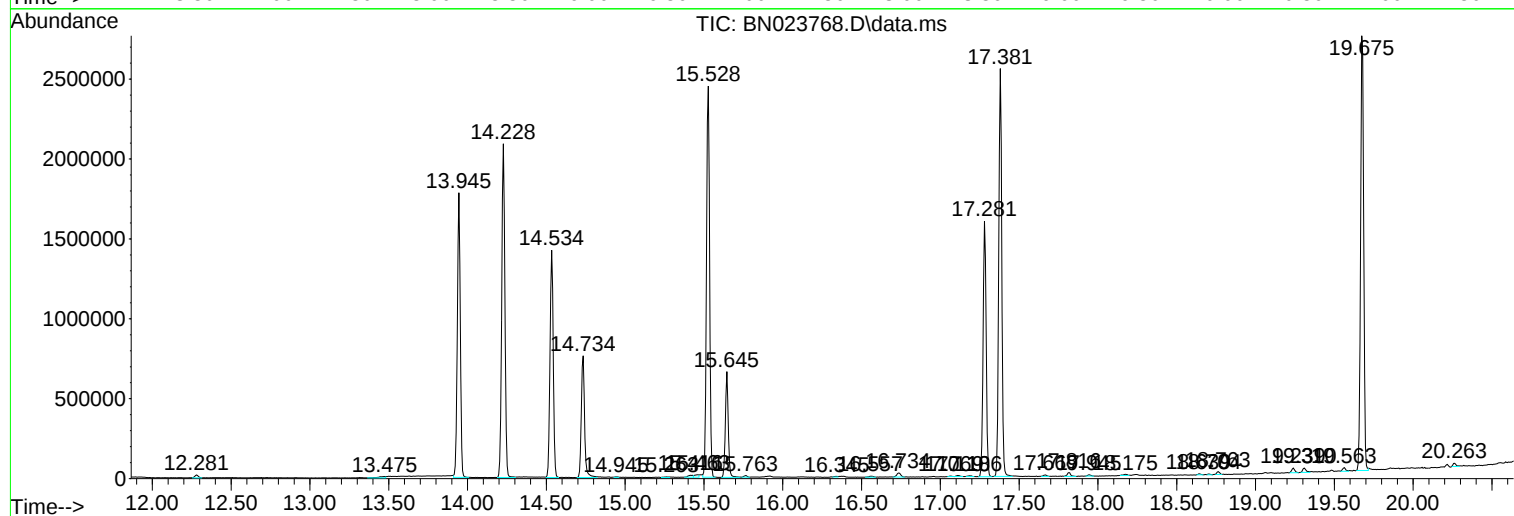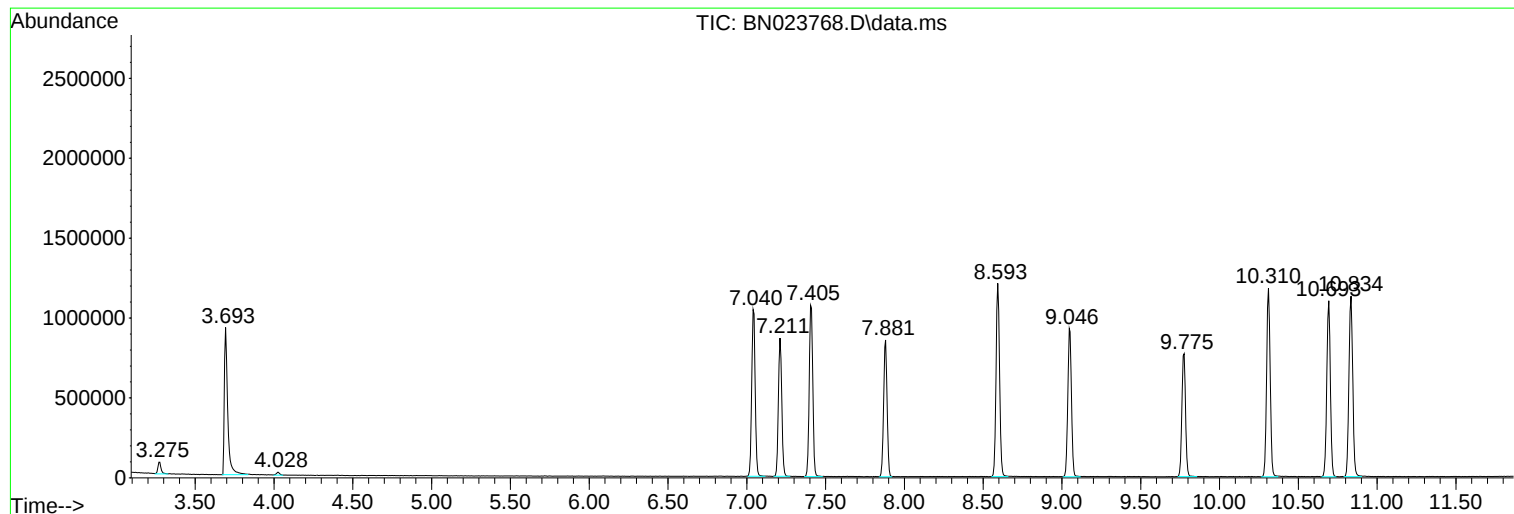

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023768.D
Acq On : 24 Jan 2023 09:34
Operator : CG/JU
Sample : PB150407BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023768.D
Acq On : 24 Jan 2023 09:34
Operator : CG/JU
Sample : PB150407BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc