

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023772.D
 Acq On : 24 Jan 2023 12:00
 Operator : CG/JU
 Sample : PB150410BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK410

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	43	rVB	62761	87299	2.04%	0.172%
2	3.693	100	103	122	rBV	802697	1162768	27.22%	2.289%
3	4.028	156	160	166	rVB	16835	24151	0.57%	0.048%
4	7.046	666	673	685	rBV	951454	1492755	34.94%	2.939%
5	7.216	696	702	714	rBV	786634	1187624	27.80%	2.338%
6	7.410	728	735	750	rBV	978135	1546817	36.21%	3.046%
7	7.887	809	816	823	rBV	891325	1358599	31.80%	2.675%
8	8.599	930	937	949	rBV	1166586	1776537	41.59%	3.498%
9	9.052	1007	1014	1027	rBV	881605	1437914	33.66%	2.831%
10	9.775	1130	1137	1147	rBV	748685	1198859	28.06%	2.361%
11	10.316	1221	1229	1239	rBV	1036332	1675349	39.22%	3.299%
12	10.698	1286	1294	1301	rBV	1033068	1703788	39.88%	3.355%
13	10.840	1310	1318	1331	rBV	993749	1660238	38.86%	3.269%
14	12.287	1559	1564	1572	rVB	17123	29112	0.68%	0.057%
15	13.945	1840	1846	1857	rBV	1932855	2536692	59.38%	4.995%
16	14.228	1887	1894	1907	rBV2	2196993	3054912	71.51%	6.015%
17	14.534	1939	1946	1956	rVB	1715510	2446176	57.26%	4.816%
18	14.734	1974	1980	2001	rBV	851614	1225604	28.69%	2.413%
19	14.898	2005	2008	2012	rVV6	3000	4743	0.11%	0.009%
20	15.528	2108	2115	2122	rBV	2691044	3712253	86.90%	7.309%
21	15.645	2129	2135	2151	rBV	778977	995503	23.30%	1.960%
22	15.763	2151	2155	2161	rVB2	11723	18087	0.42%	0.036%
23	17.069	2373	2377	2382	rVB3	3870	5102	0.12%	0.010%
24	17.280	2407	2413	2422	rBV	2069536	2830648	66.26%	5.573%
25	17.380	2423	2430	2441	rBV	2888868	3942744	92.30%	7.763%
26	19.239	2742	2746	2752	rVB3	30901	41585	0.97%	0.082%
27	19.304	2754	2757	2763	rBV	28481	39649	0.93%	0.078%
28	19.674	2814	2820	2831	rBV	3283196	4271810	100.00%	8.411%
29	21.474	3121	3126	3136	rBV	2065966	2638638	61.77%	5.195%
30	23.739	3504	3511	3524	rBV2	1946147	3953129	92.54%	7.784%
31	23.892	3530	3537	3546	rBV2	1491798	2729216	63.89%	5.374%




Sum of corrected areas: 50788301

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023772.D
Acq On : 24 Jan 2023 12:00
Operator : CG/JU
Sample : PB150410BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

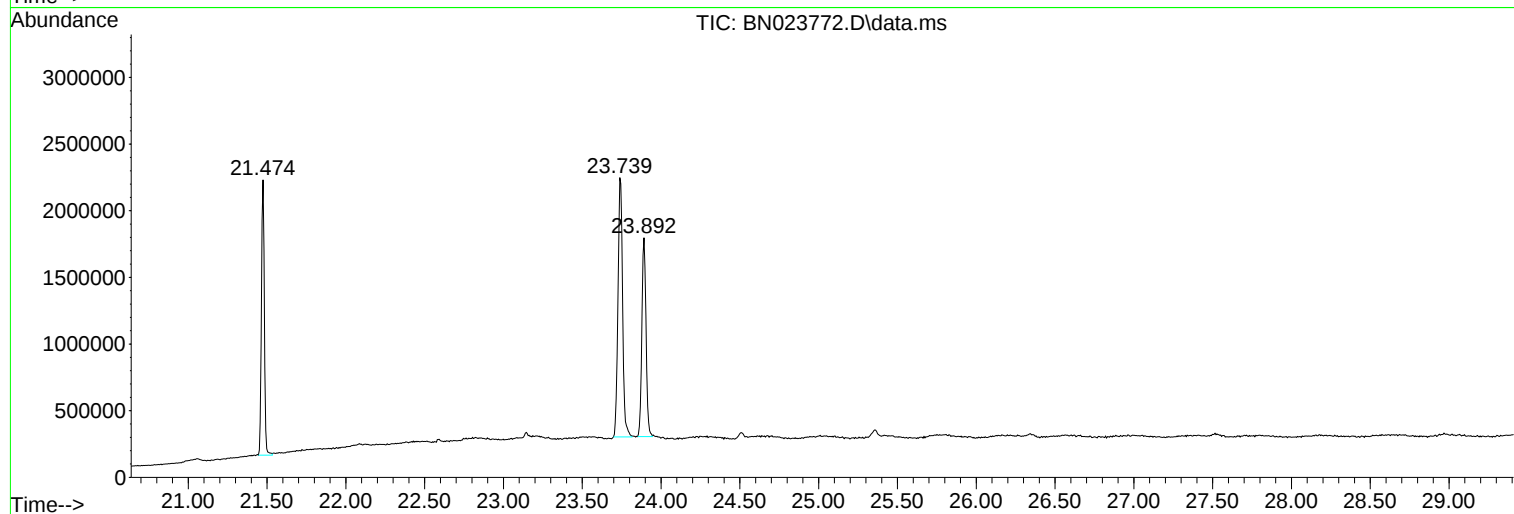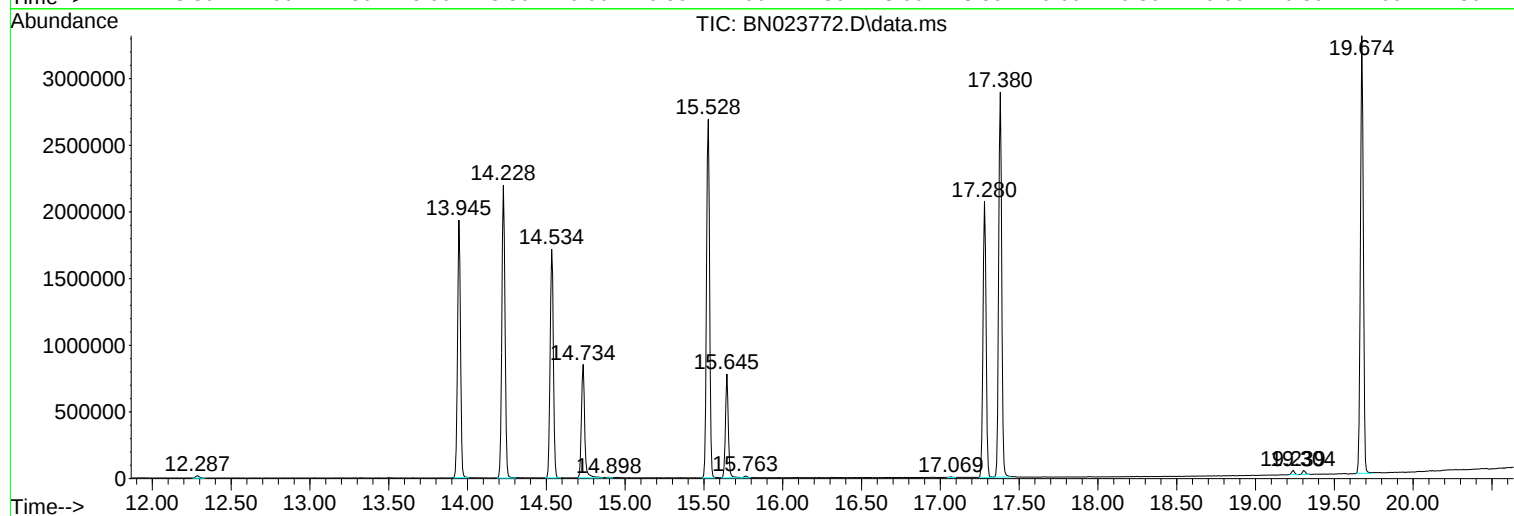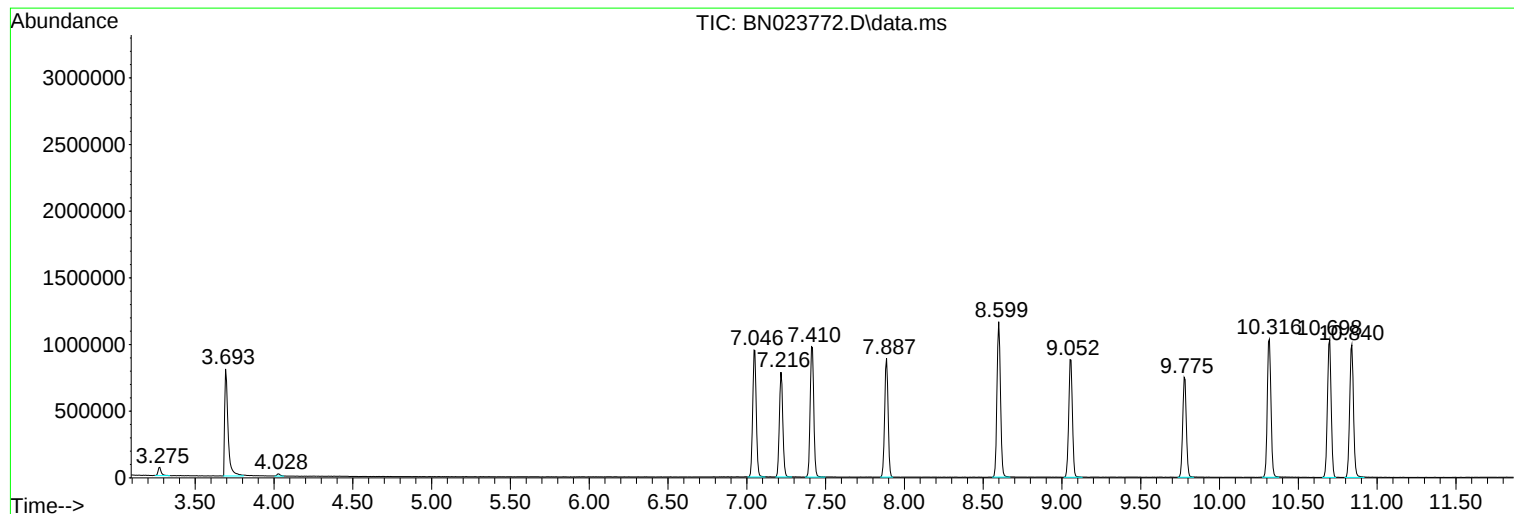

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023772.D
Acq On : 24 Jan 2023 12:00
Operator : CG/JU
Sample : PB150410BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023772.D
Acq On : 24 Jan 2023 12:00
Operator : CG/JU
Sample : PB150410BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc