

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023785.D
 Acq On : 24 Jan 2023 20:05
 Operator : CG/JU
 Sample : PB150438BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK438

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	38	rVB	53518	70928	1.61%	0.157%
2	3.693	101	103	131	rBV	514618	799099	18.16%	1.767%
3	4.028	156	160	169	rVB	16971	24421	0.55%	0.054%
4	7.052	666	674	685	rBV	771553	1170042	26.59%	2.588%
5	7.216	696	702	712	rVB	614057	918291	20.87%	2.031%
6	7.416	729	736	745	rBV	835329	1273185	28.93%	2.816%
7	7.887	809	816	824	rBV	718259	1087189	24.70%	2.405%
8	8.599	930	937	951	rBV	921166	1415697	32.17%	3.131%
9	9.057	1008	1015	1026	rVB	760596	1208120	27.45%	2.672%
10	9.781	1130	1138	1145	rBV	673488	1088599	24.74%	2.408%
11	10.316	1221	1229	1241	rBV	1030244	1644675	37.37%	3.638%
12	10.698	1286	1294	1302	rVB	1079243	1795647	40.80%	3.972%
13	10.840	1311	1318	1332	rBV	778986	1304362	29.64%	2.885%
14	12.287	1559	1564	1571	rVB	15575	23190	0.53%	0.051%
15	13.945	1840	1846	1859	rVB	1633982	2227584	50.62%	4.927%
16	14.228	1887	1894	1907	rBV	1820865	2603285	59.15%	5.758%
17	14.534	1939	1946	1954	rBV	1376706	1983089	45.06%	4.386%
18	14.734	1974	1980	1996	rBV	727891	1067281	24.25%	2.361%
19	15.528	2108	2115	2122	rBV	2222347	3029753	68.84%	6.701%
20	15.645	2129	2135	2146	rBV	721667	941161	21.39%	2.082%
21	15.769	2151	2156	2161	rVB	11055	16154	0.37%	0.036%
22	17.280	2407	2413	2423	rVB	1723477	2373464	53.93%	5.250%
23	17.380	2423	2430	2446	rBV	2419579	3283480	74.61%	7.262%
24	17.951	2523	2527	2531	rBV6	6179	8764	0.20%	0.019%
25	19.239	2742	2746	2752	rBV4	30954	42793	0.97%	0.095%
26	19.310	2754	2758	2762	rVB	29512	36917	0.84%	0.082%
27	19.674	2814	2820	2829	rBV	3437471	4400995	100.00%	9.734%
28	21.468	3120	3125	3133	rBV	2322449	2861367	65.02%	6.329%
29	23.733	3502	3510	3524	rVB	1886148	3980133	90.44%	8.803%
30	23.892	3531	3537	3549	rVB2	1360874	2532858	57.55%	5.602%




Sum of corrected areas: 45212523

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023785.D
Acq On : 24 Jan 2023 20:05
Operator : CG/JU
Sample : PB150438BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

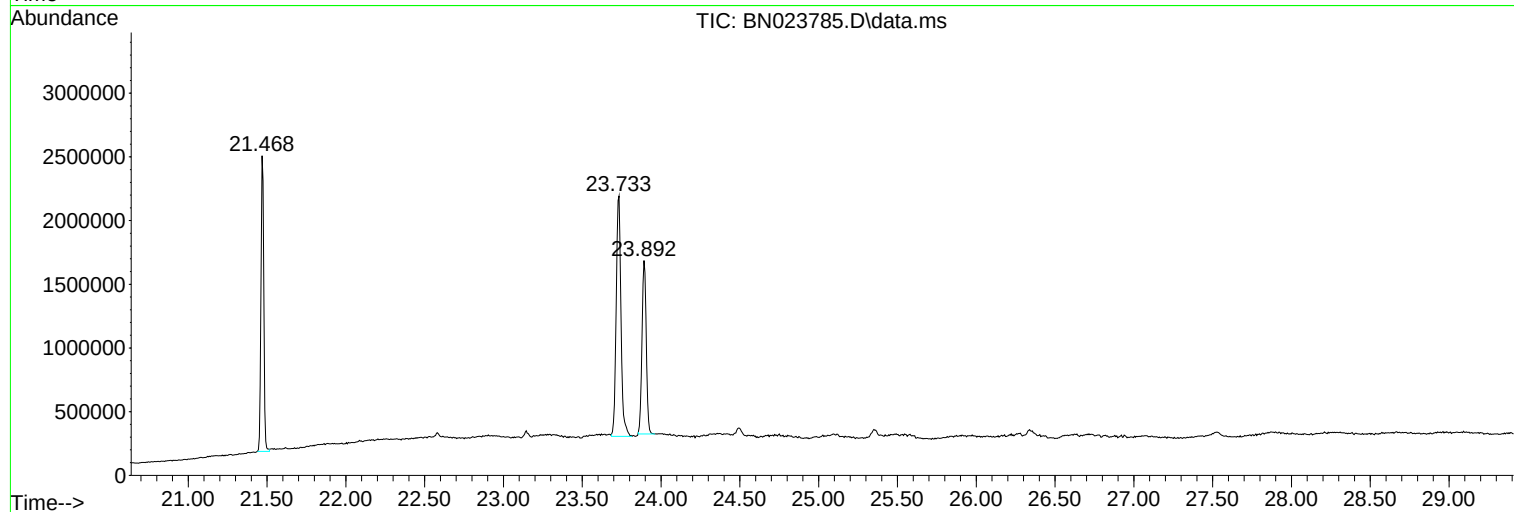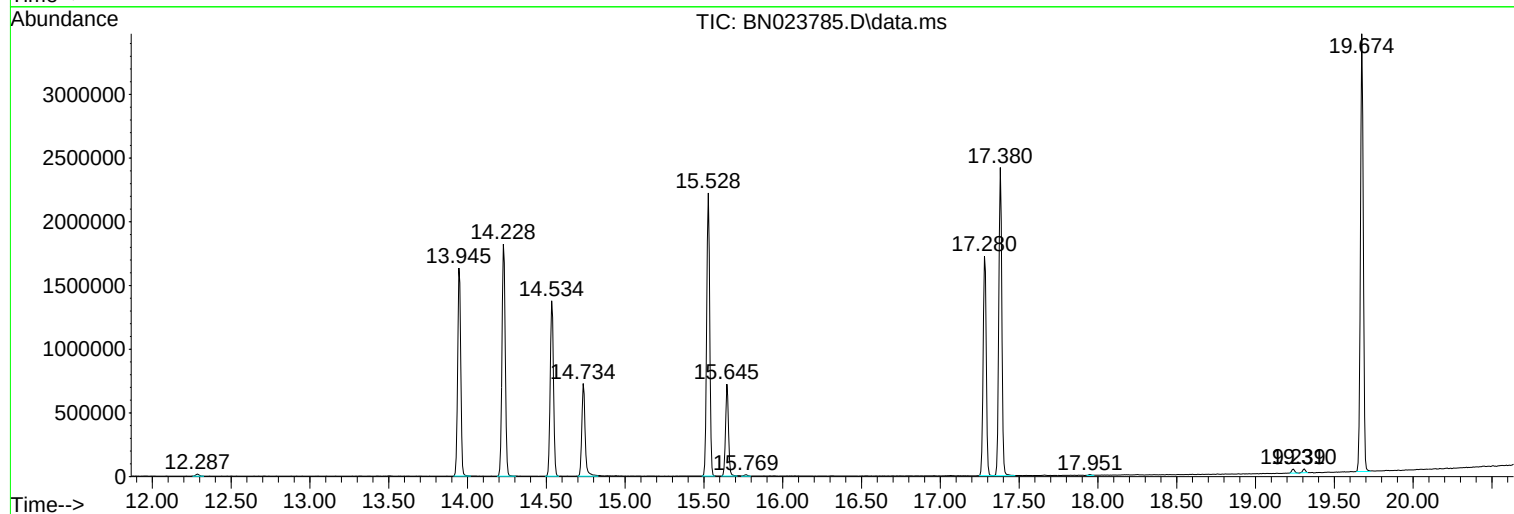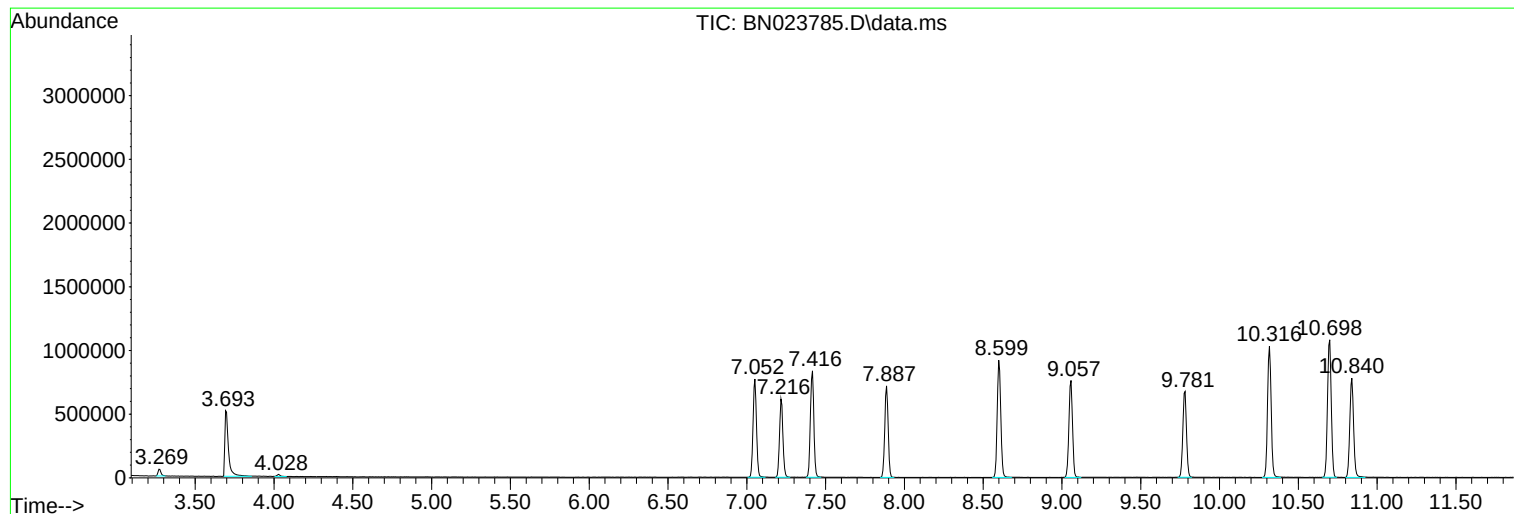

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023785.D
Acq On : 24 Jan 2023 20:05
Operator : CG/JU
Sample : PB150438BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023785.D
Acq On : 24 Jan 2023 20:05
Operator : CG/JU
Sample : PB150438BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc