

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
 Data File : BN036044.D
 Acq On : 27 Jan 2025 19:37
 Operator : RC/JU
 Sample : Q1174-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2945

Quant Time: Jan 28 00:08:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.812	152	2832	0.400	ng/ul	0.00
4) Naphthalene-d8	10.604	136	6091	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.449	164	3643	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.368	240	5965	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.67
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.272	96	15615	5.036	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.193	152	2564	0.333	ng/ul	0.00
18) Fluoranthene-d10	19.219	212	6948	0.424	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.444	166	1109	0.079	ng/ul#	15
20) Pyrene	19.582	202	1100	0.046	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036044.D
Acq On : 27 Jan 2025 19:37
Operator : RC/JU
Sample : Q1174-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2945

Quant Time: Jan 28 00:08:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration




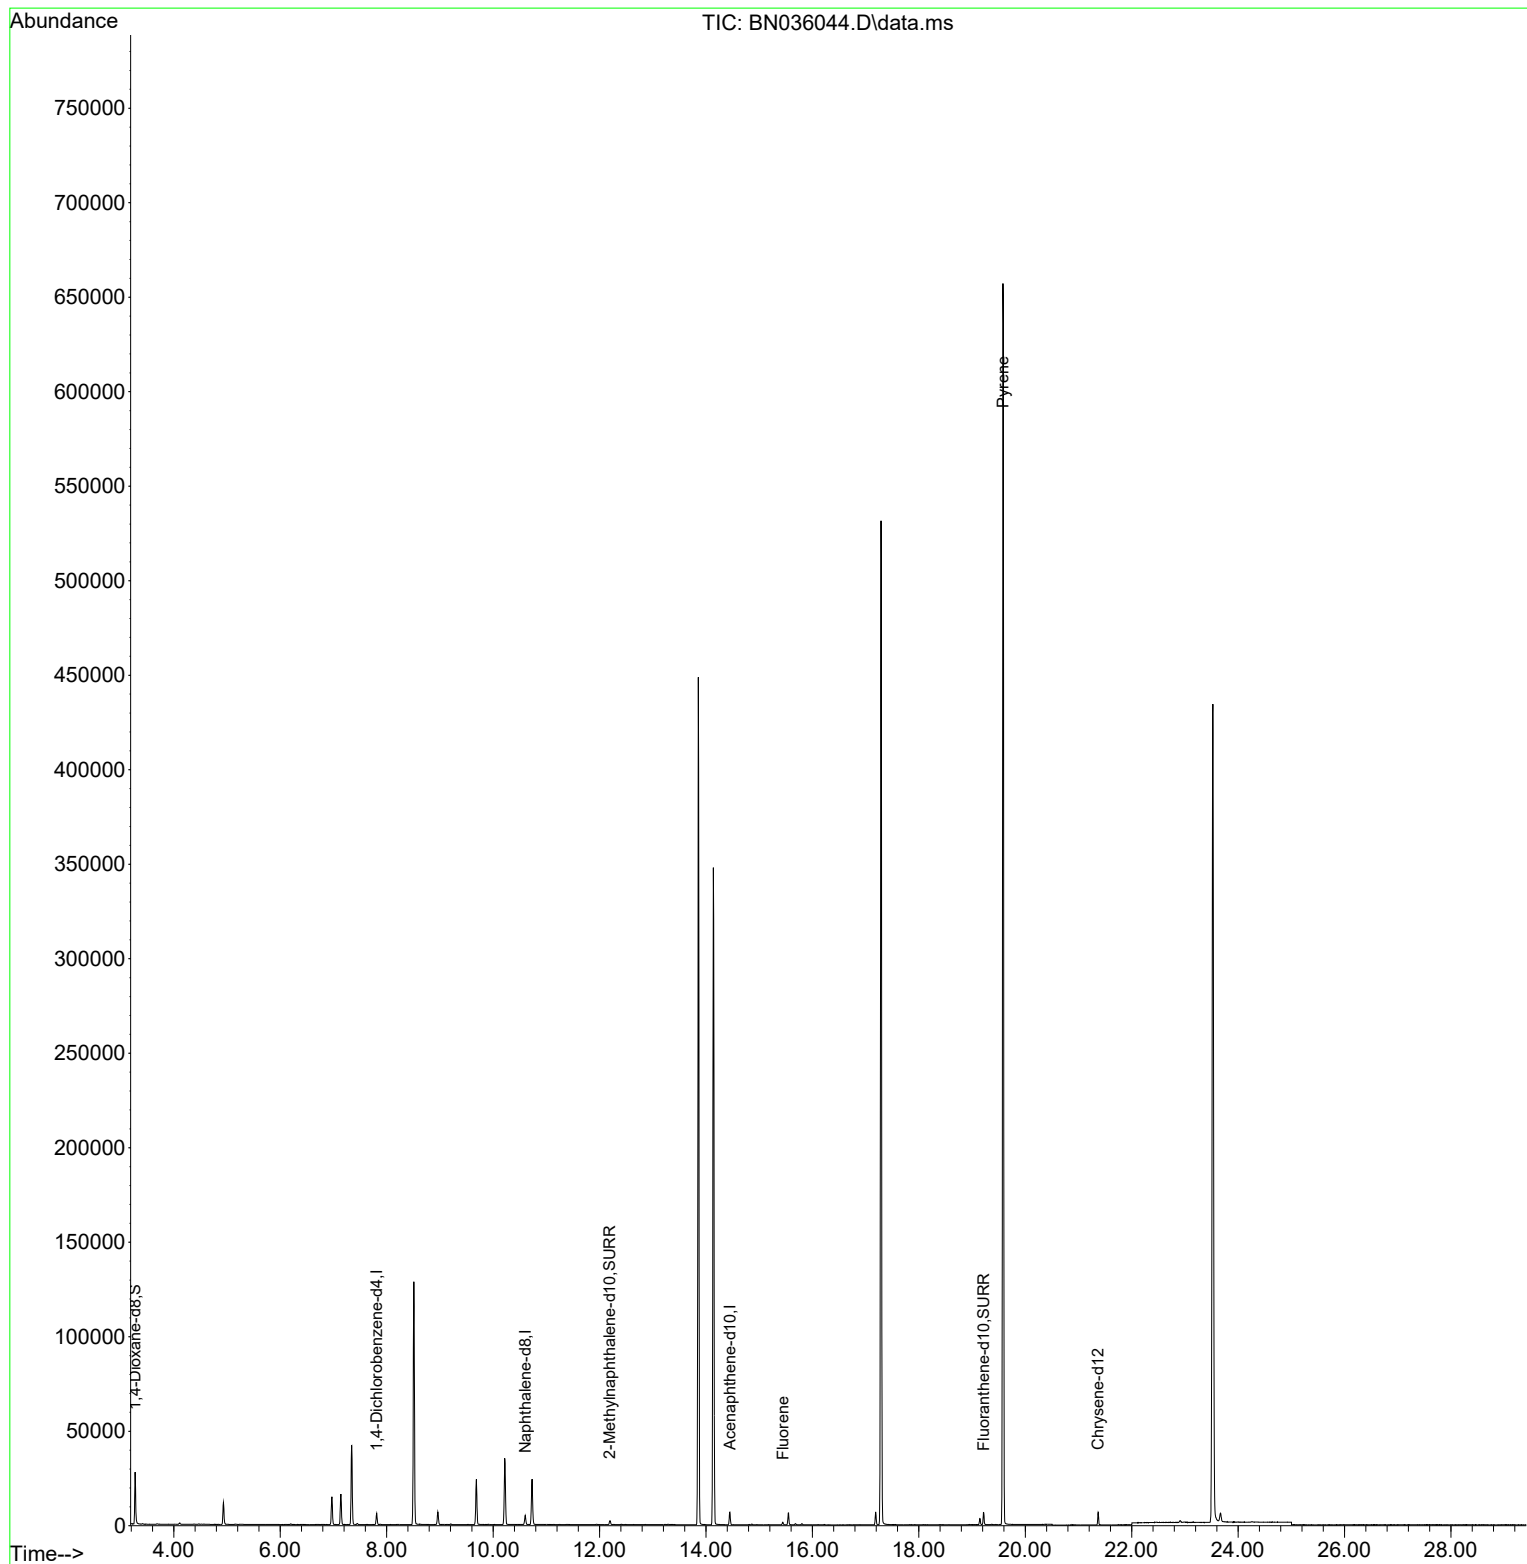


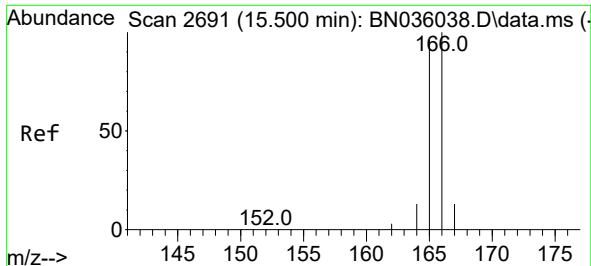

#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.444 min Scan# 20
Delta R.T. -0.056 min
Lab File: BN036044.D
Acq: 27 Jan 2025 19:37

Instrument :
BNA_N
ClientSampleId :
E2945

Tgt Ion:166 Resp: 1109
Ion Ratio Lower Upper
166 100
165 10.7 80.3 120.5#
167 40.0 12.3 18.5#

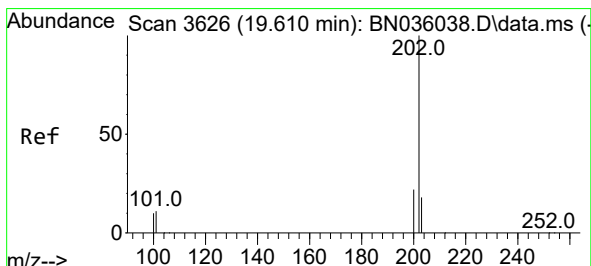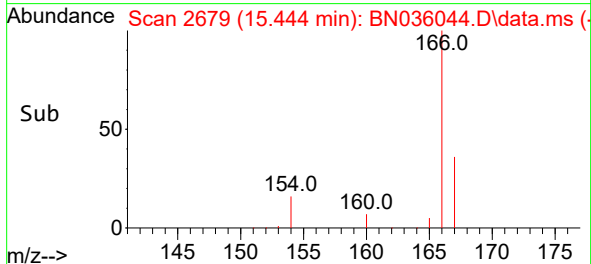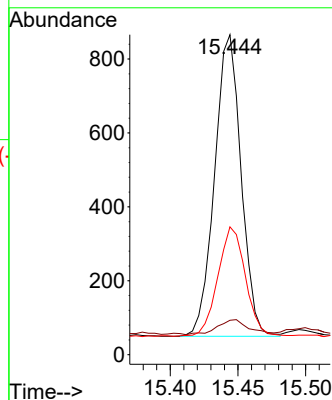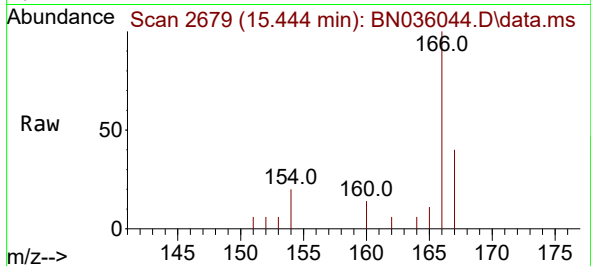

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.582 min Scan# 3620
Delta R.T. -0.028 min
Lab File: BN036044.D
Acq: 27 Jan 2025 19:37

Tgt Ion:202 Resp: 1100
Ion Ratio Lower Upper
202 100
101 230.1 9.3 13.9#
100 1797.3 7.5 11.3#

