

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
 Data File : BN036045.D
 Acq On : 27 Jan 2025 20:13
 Operator : RC/JU
 Sample : Q1174-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2950

Quant Time: Jan 28 00:08:57 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	2683	0.400	ng/ul	0.00
4) Naphthalene-d8	10.605	136	5915	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	3583	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.371	240	5696	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.67
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.272	96	11777	4.009	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.194	152	2688	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.219	212	6767	0.432	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.582	202	1093	0.048	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036045.D
Acq On : 27 Jan 2025 20:13
Operator : RC/JU
Sample : Q1174-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2950


Quant Time: Jan 28 00:08:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

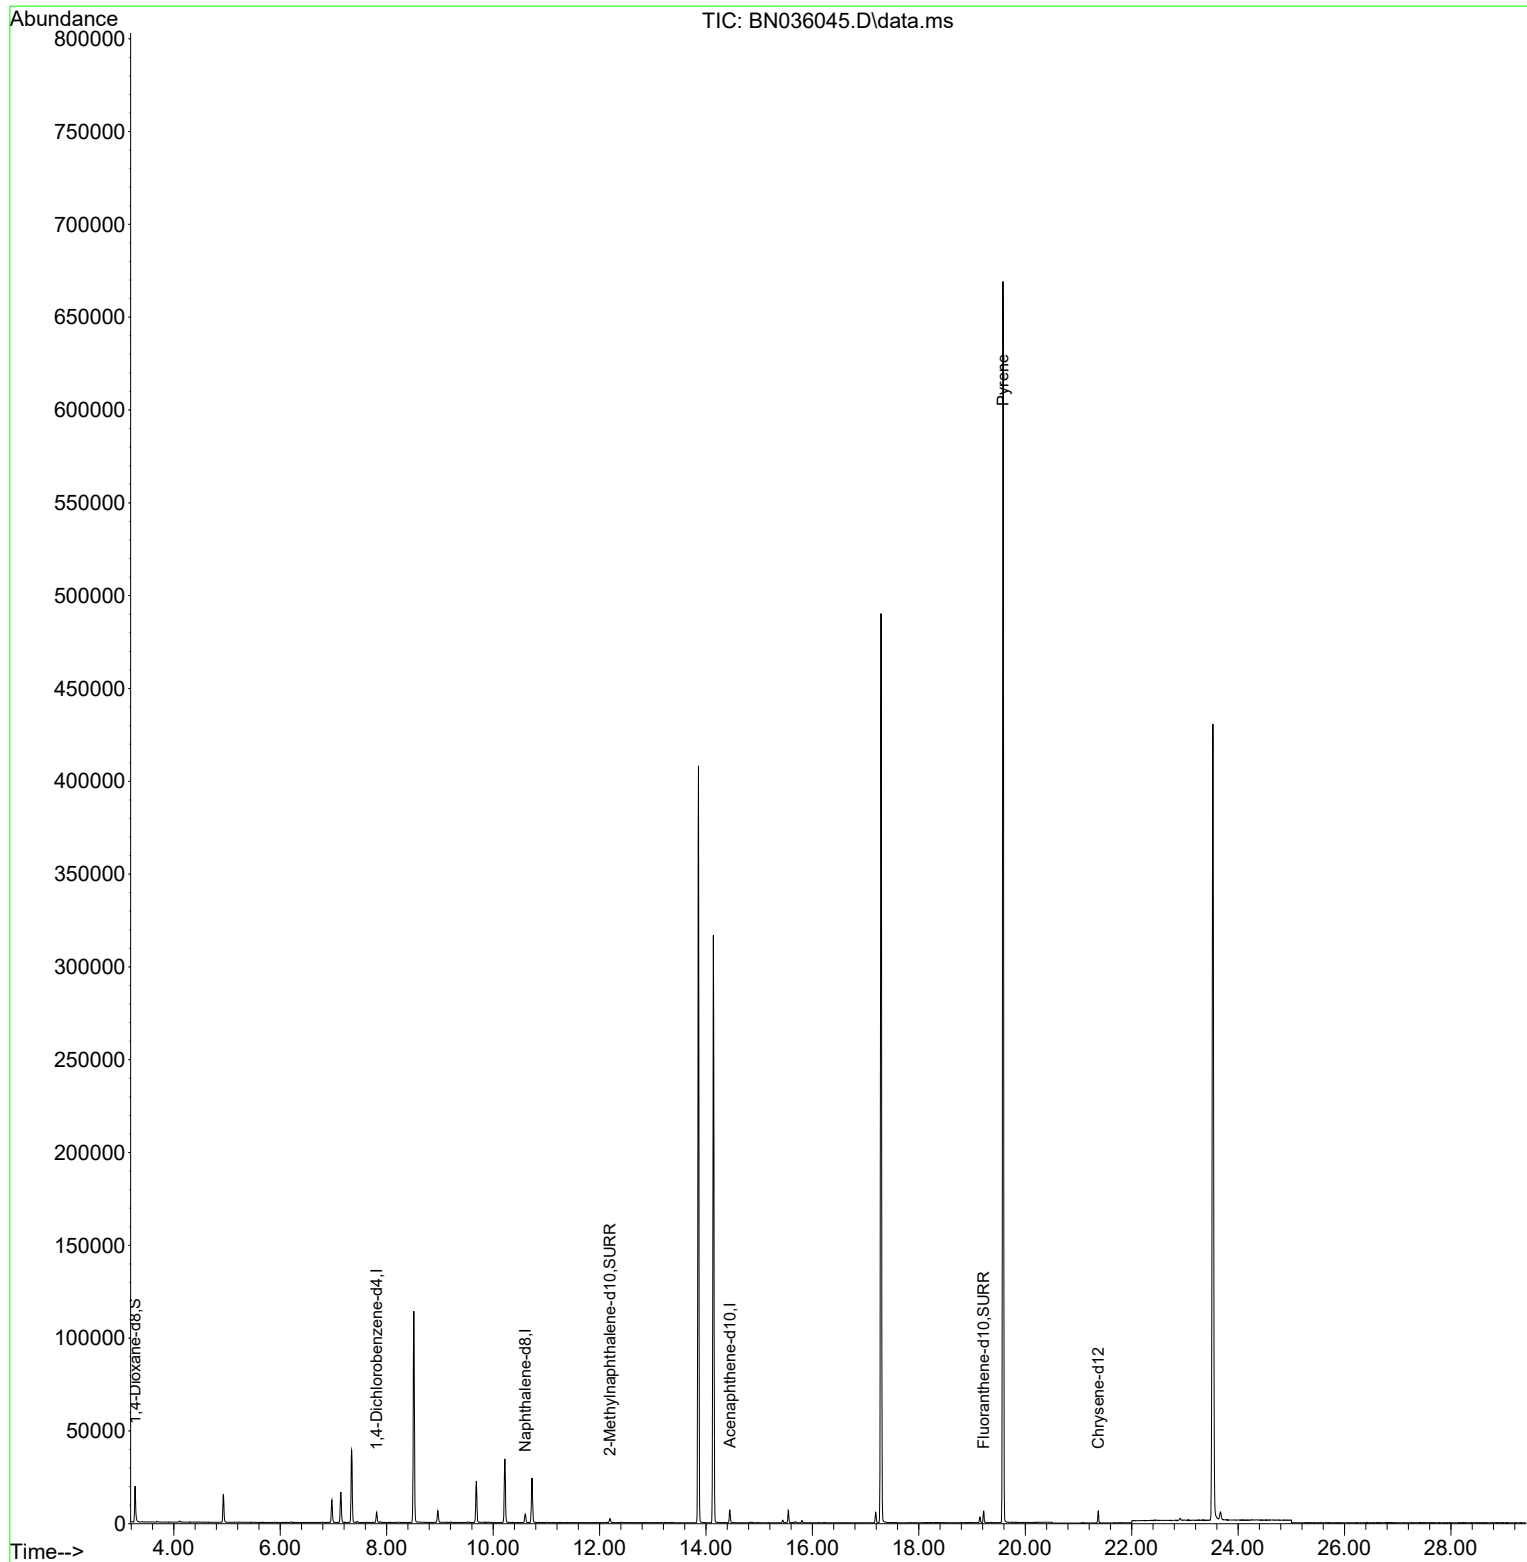

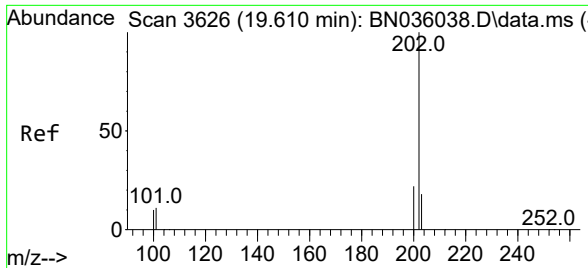

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.582 min Scan# 30
Delta R.T. -0.028 min
Lab File: BN036045.D
Acq: 27 Jan 2025 20:13

Instrument :
BNA_N
ClientSampleId :
E2950

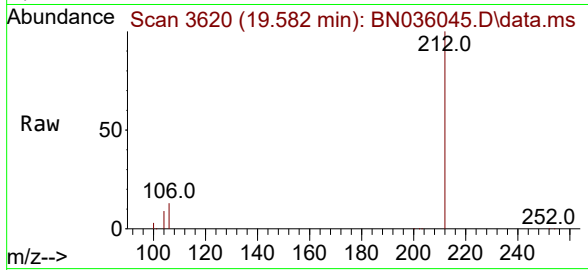

Tgt Ion:202 Resp: 1093
Ion Ratio Lower Upper
202 100
101 212.5 9.3 13.9#
100 1626.2 7.5 11.3#

