




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036046.D
Acq On : 27 Jan 2025 20:49
Operator : RC/JU
Sample : Q1174-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2951

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2025
Supervised By :mohammad ahmed 01/31/2025

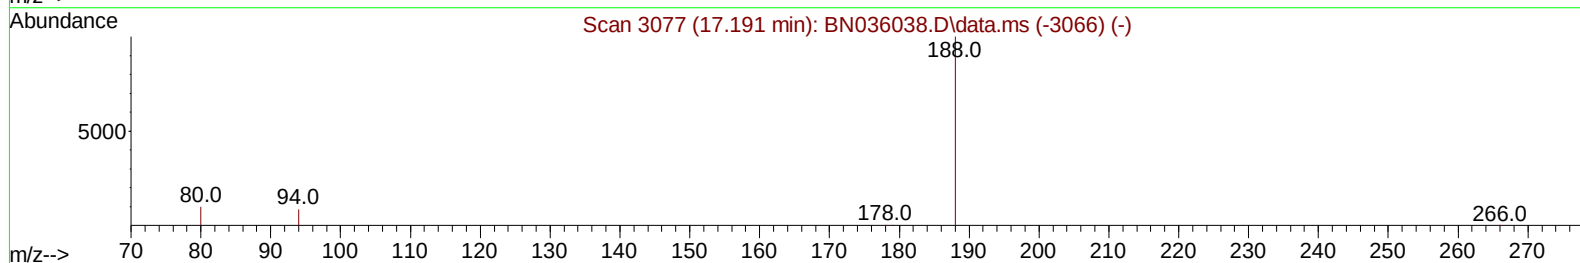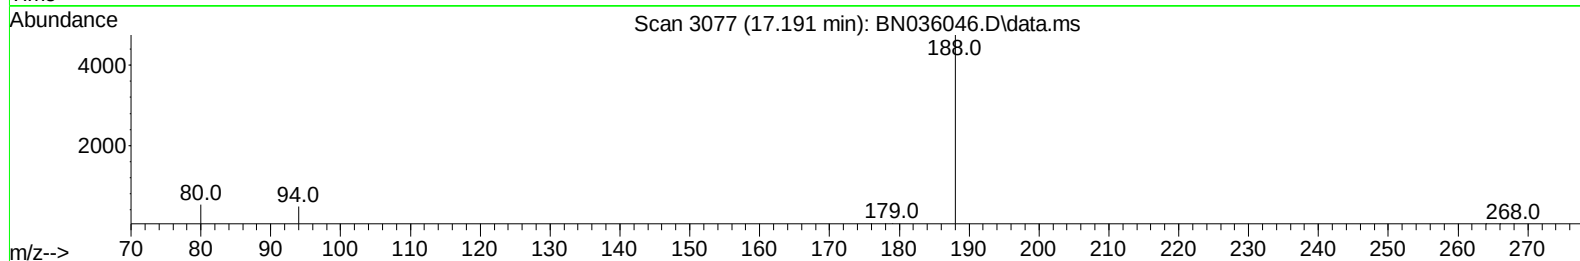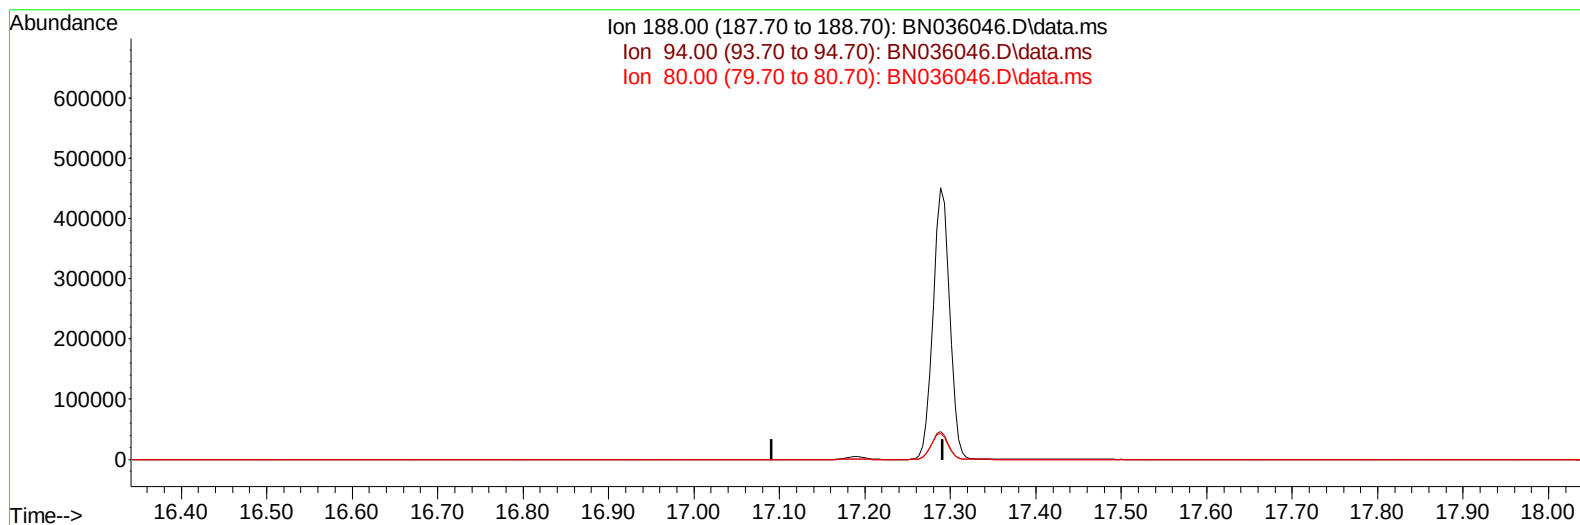

TIC: BN036046.D\data.ms

(13) Phenanthrene-d10 (I)

17.191min (-17.191) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.10	0.00#
80.00	10.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036046.D
Acq On : 27 Jan 2025 20:49
Operator : RC/JU
Sample : Q1174-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2951

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2025
Supervised By :mohammad ahmed 01/31/2025

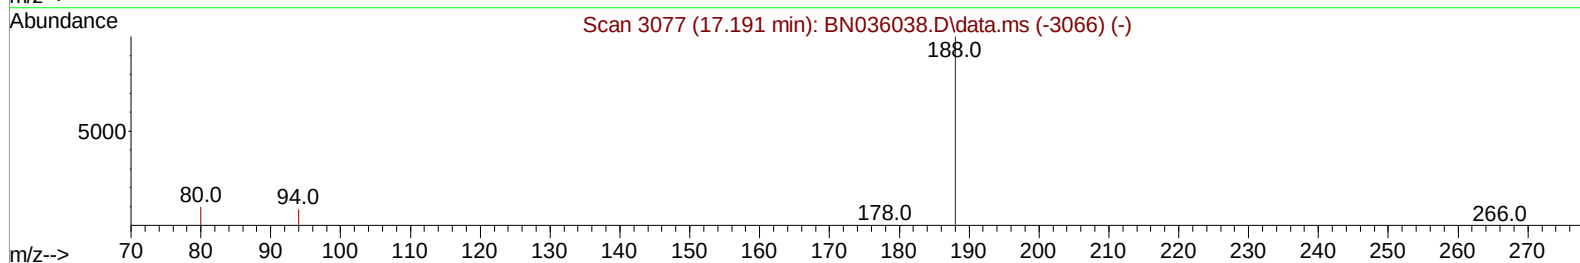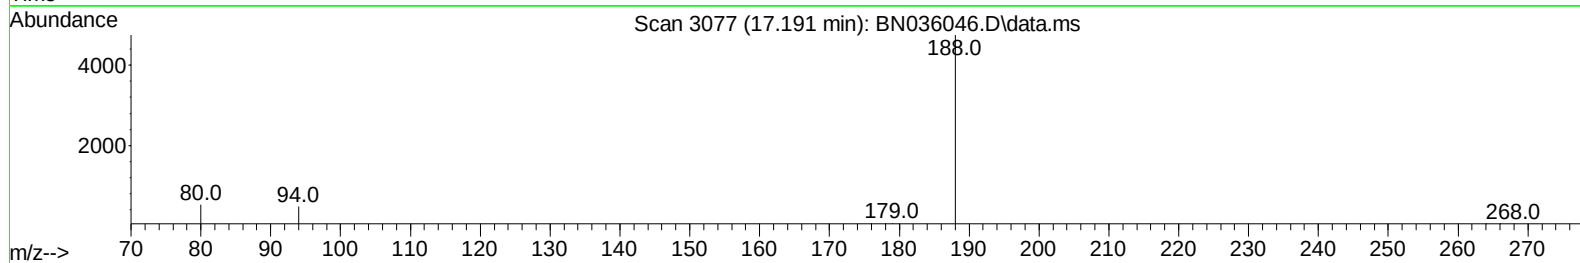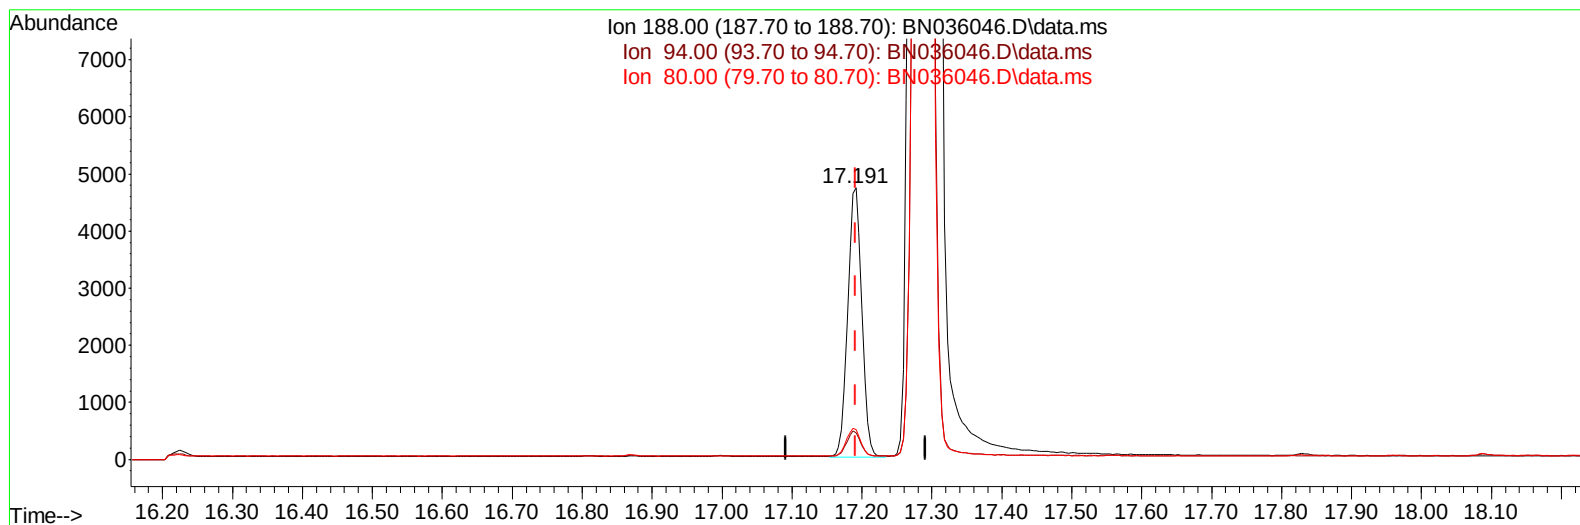

TIC: BN036046.D\data.ms

(13) Phenanthrene-d10 (I)

17.191min (+ 0.000) 0.40 ng/ul m

response 6625

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	9.88
80.00	10.90	10.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036046.D
Acq On : 27 Jan 2025 20:49
Operator : RC/JU
Sample : Q1174-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2951

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/28/2025
Supervised By :mohammad ahmed 01/31/2025

Quant Time: Jan 28 00:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

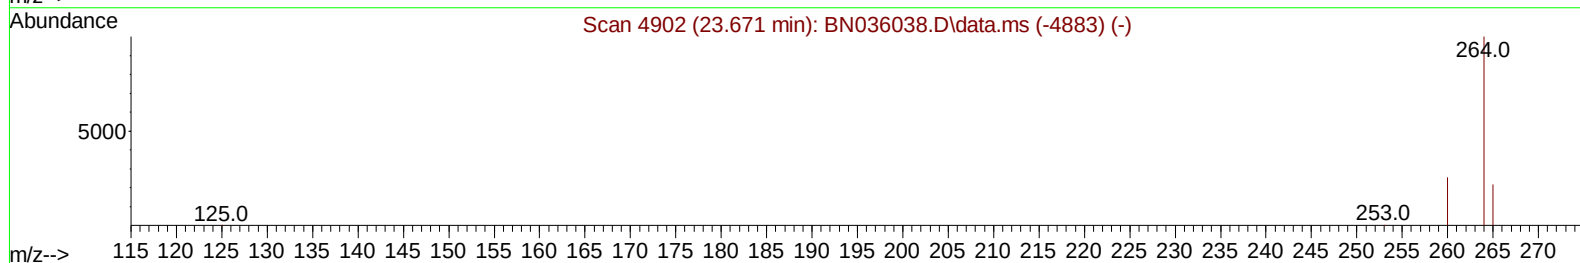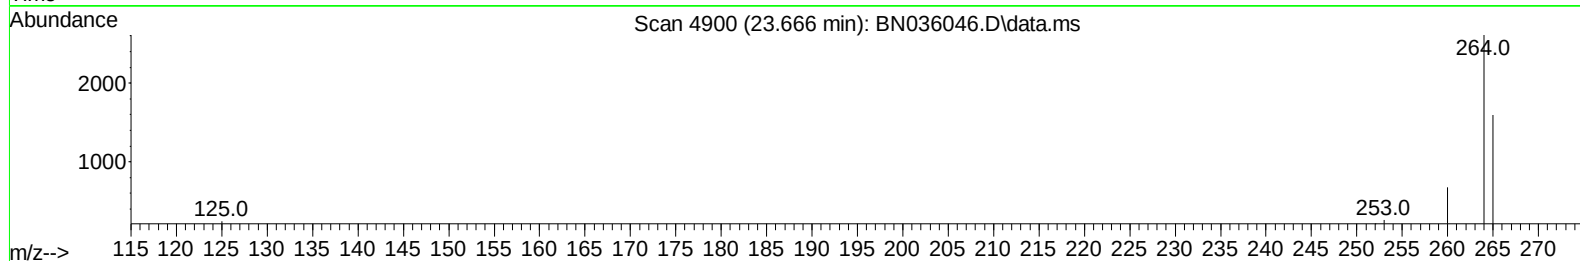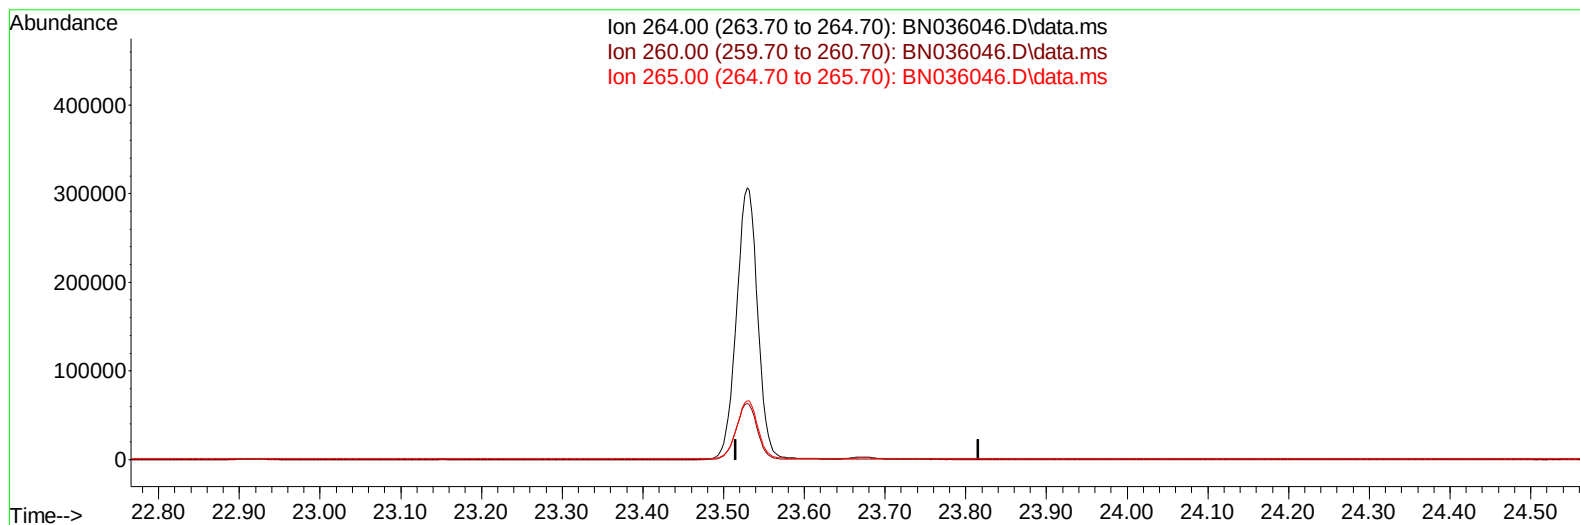

TIC: BN036046.D\data.ms

(23) Perylene-d12 (I)

23.666min (-23.666) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.80	0.00#
265.00	53.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036046.D
Acq On : 27 Jan 2025 20:49
Operator : RC/JU
Sample : Q1174-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2951

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2025
Supervised By :mohammad ahmed 01/31/2025

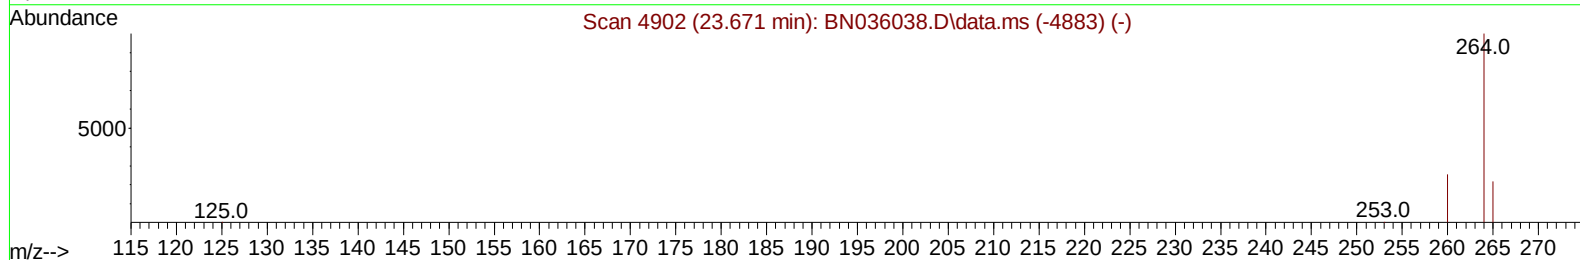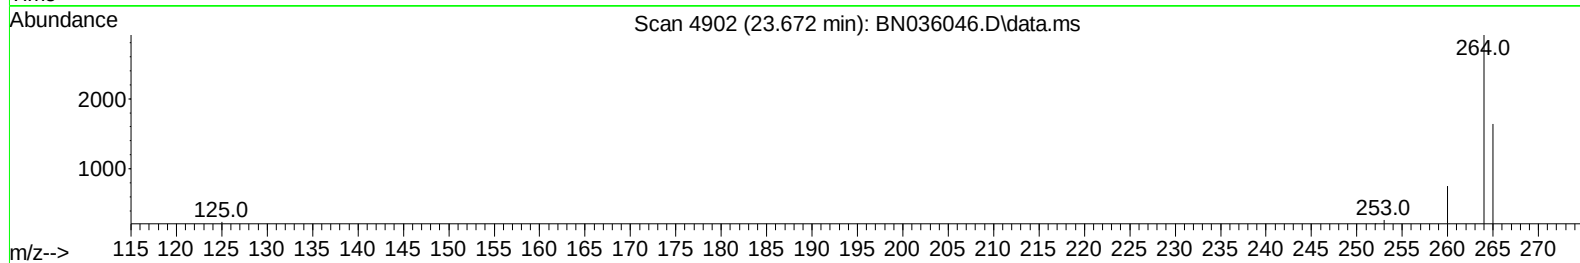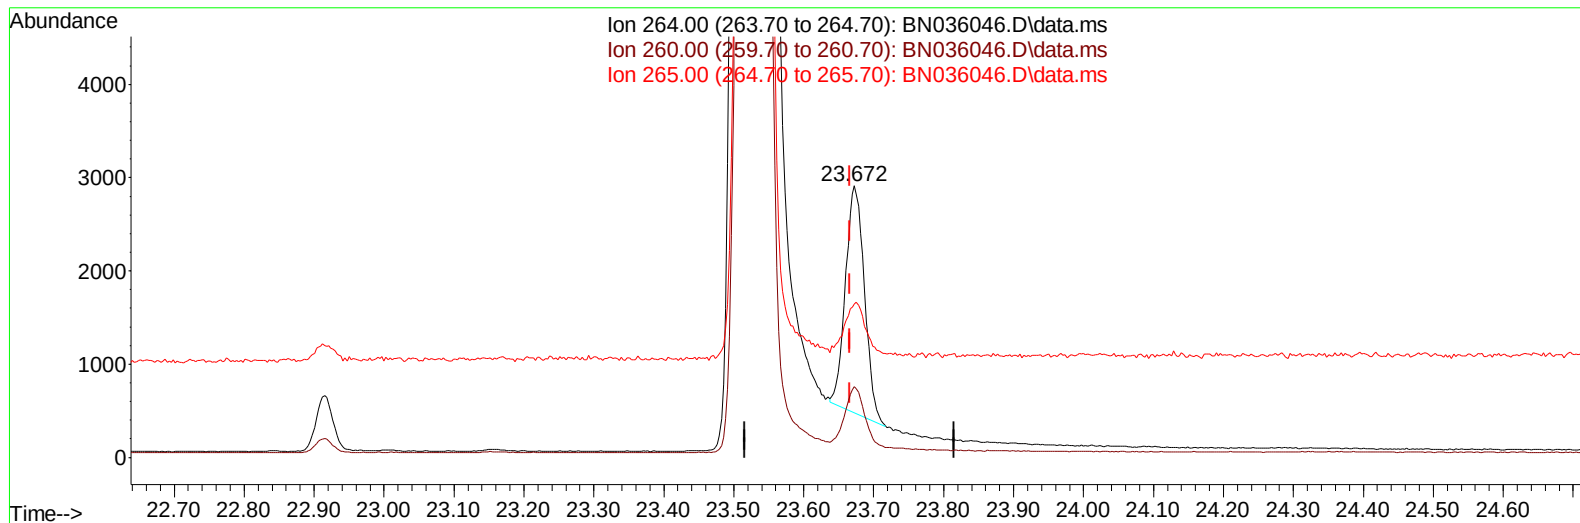

TIC: BN036046.D\data.ms

(23) Perylene-d12 (I)

23.672min (+ 0.007) 0.40 ng/ul m

response 4561

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.04
265.00	53.20	56.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
 Data File : BN036046.D
 Acq On : 27 Jan 2025 20:49
 Operator : RC/JU
 Sample : Q1174-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2951

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/28/2025
 Supervised By :mohammad ahmed 01/31/2025

Quant Time: Jan 28 00:09:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.812	152	2653	0.400	ng/ul	0.00
4) Naphthalene-d8	10.605	136	5877	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	3604	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.191	188	6625m	0.400	ng/ul	0.00
17) Chrysene-d12	21.372	240	5260	0.400	ng/ul	0.00
23) Perylene-d12	23.672	264	4561m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.272	96	14634	5.038	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.194	152	3037	0.409	ng/ul	0.00
18) Fluoranthene-d10	19.215	212	7242	0.501	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012725\
Data File : BN036046.D
Acq On : 27 Jan 2025 20:49
Operator : RC/JU
Sample : Q1174-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2951

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/28/2025
Supervised By :mohammad ahmed 01/31/2025

