

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
 Data File : BN023863.D
 Acq On : 31 Jan 2023 16:10
 Operator : CG/JU
 Sample : 01278-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9H1

Quant Time: Jan 31 16:49:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 02:08:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	3795	0.400	ng/ul	0.00
4) Naphthalene-d8	10.667	136	10972	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.511	164	8433	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.259	188	16422	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.455	240	14154	0.400	ng/ul	# 0.00
23) Perylene-d12	23.843	264	12095	0.400	ng/ul	# 0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.243	96	18072	4.442	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.262	152	6396	0.373	ng/ul	0.00
18) Fluoranthene-d10	19.290	212	15041	0.396	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.281	88	938	0.218	ng/ul#	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
Data File : BN023863.D
Acq On : 31 Jan 2023 16:10
Operator : CG/JU
Sample : 01278-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9H1

Quant Time: Jan 31 16:49:36 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 31 02:08:51 2023
Response via : Initial Calibration

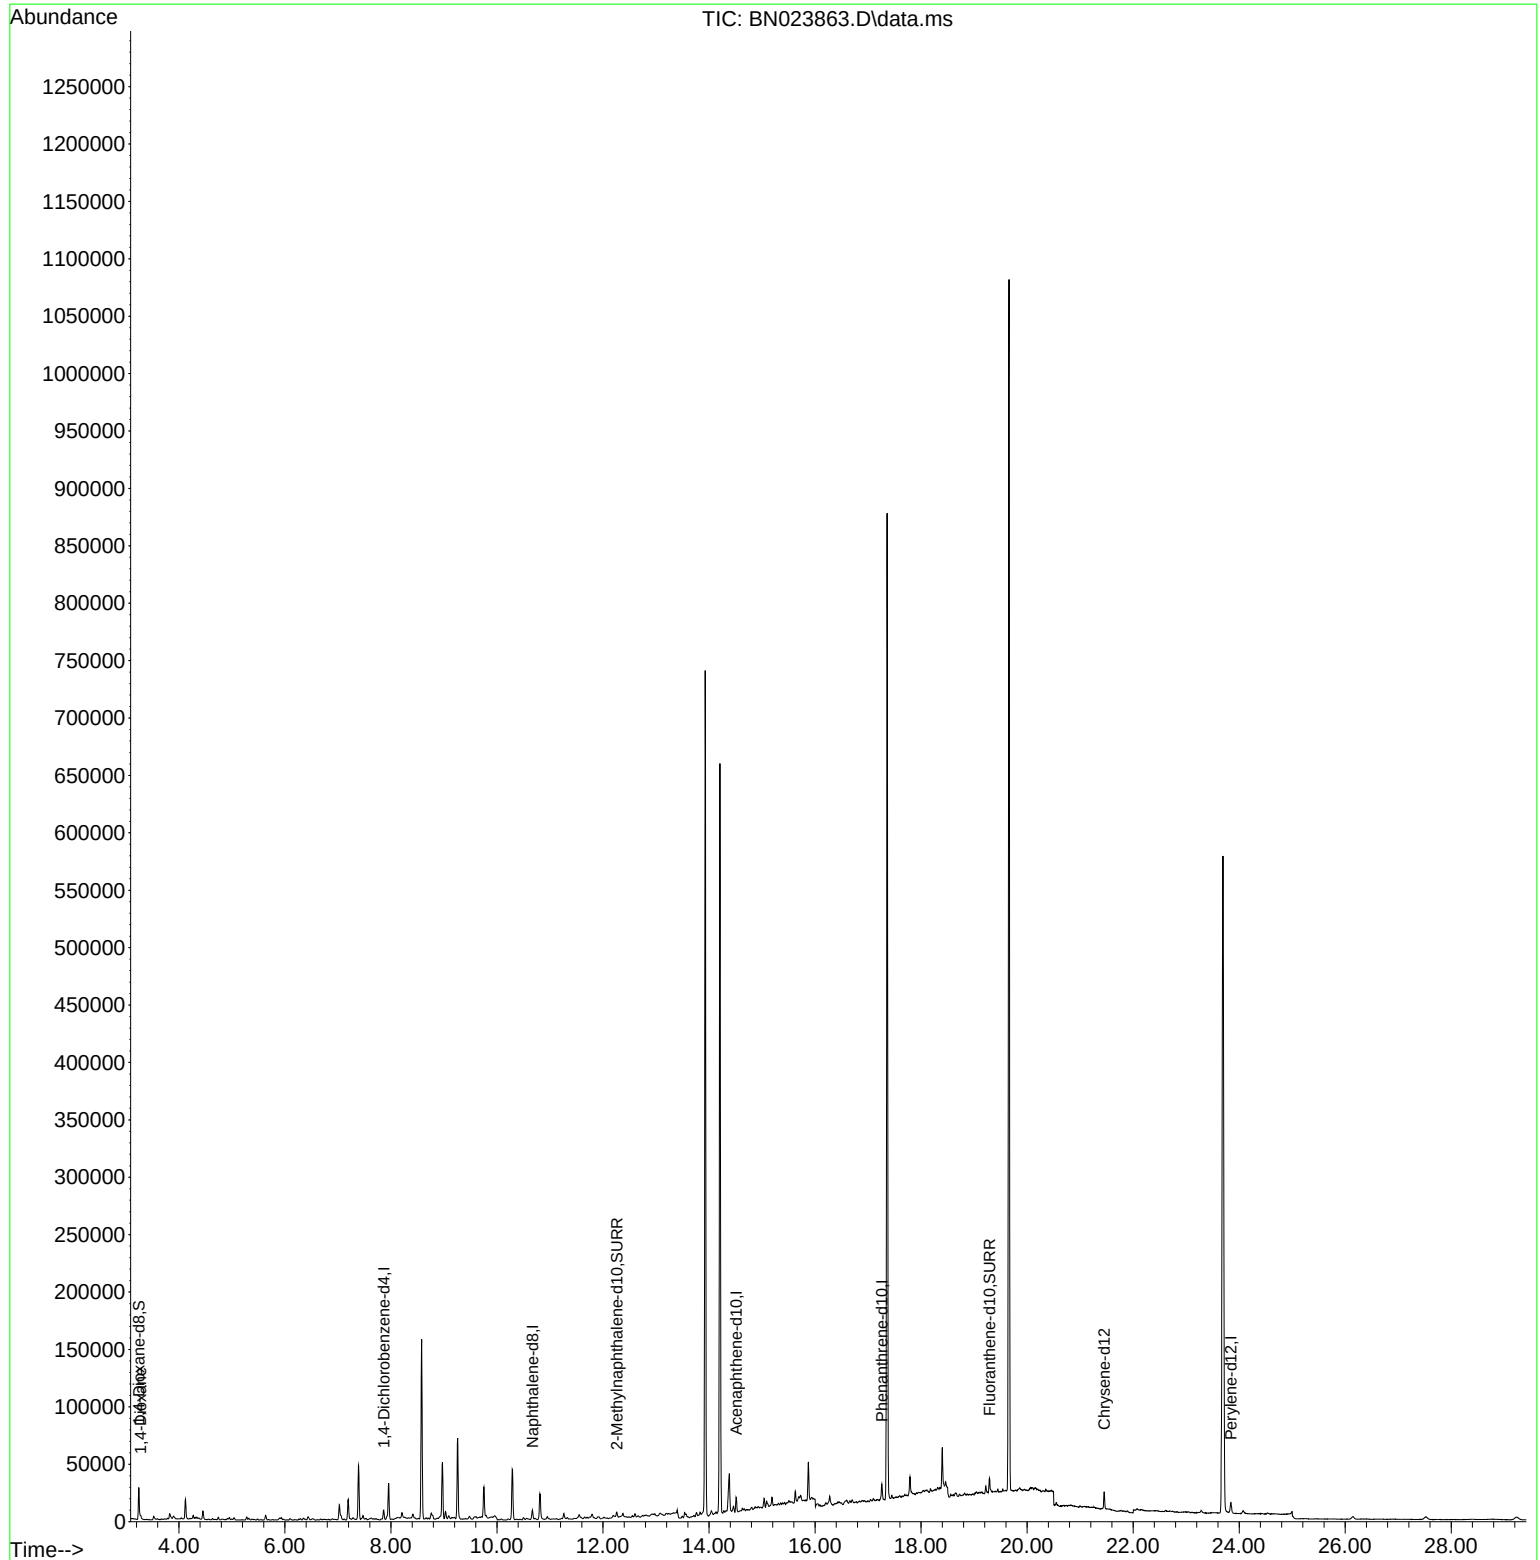

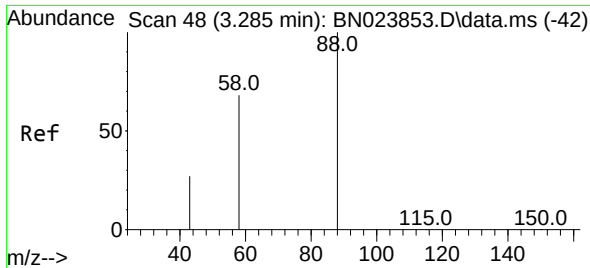

#2
 1,4-Dioxane
 Concen: 0.218 ng/ul
 RT: 3.281 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN023863.D
 Acq: 31 Jan 2023 16:10

Instrument :
 BNA_N
 ClientSampleId :
 EX9H1

Tgt Ion: 88 Resp: 938
 Ion Ratio Lower Upper
 88 100
 43 179.1 41.9 62.9#
 58 66.0 45.6 68.4

