

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
 Data File : BN023871.D
 Acq On : 31 Jan 2023 21:07
 Operator : CG/JU
 Sample : 01277-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9H3

Quant Time: Feb 01 01:05:45 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 01 01:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	4874	0.400	ng/ul	0.00
4) Naphthalene-d8	10.667	136	13559	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.511	164	8755	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.259	188	19562	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.452	240	15048	0.400	ng/ul	# 0.00
23) Perylene-d12	23.858	264	12226	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	22979	4.398	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.256	152	7253	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.285	212	18089	0.447	ng/ul	0.00
Target Compounds						
16) Anthracene	17.390	178	3238	0.066	ng/ul#	Qvalue 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
Data File : BN023871.D
Acq On : 31 Jan 2023 21:07
Operator : CG/JU
Sample : 01277-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9H3


Quant Time: Feb 01 01:05:45 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:00:14 2023
Response via : Initial Calibration

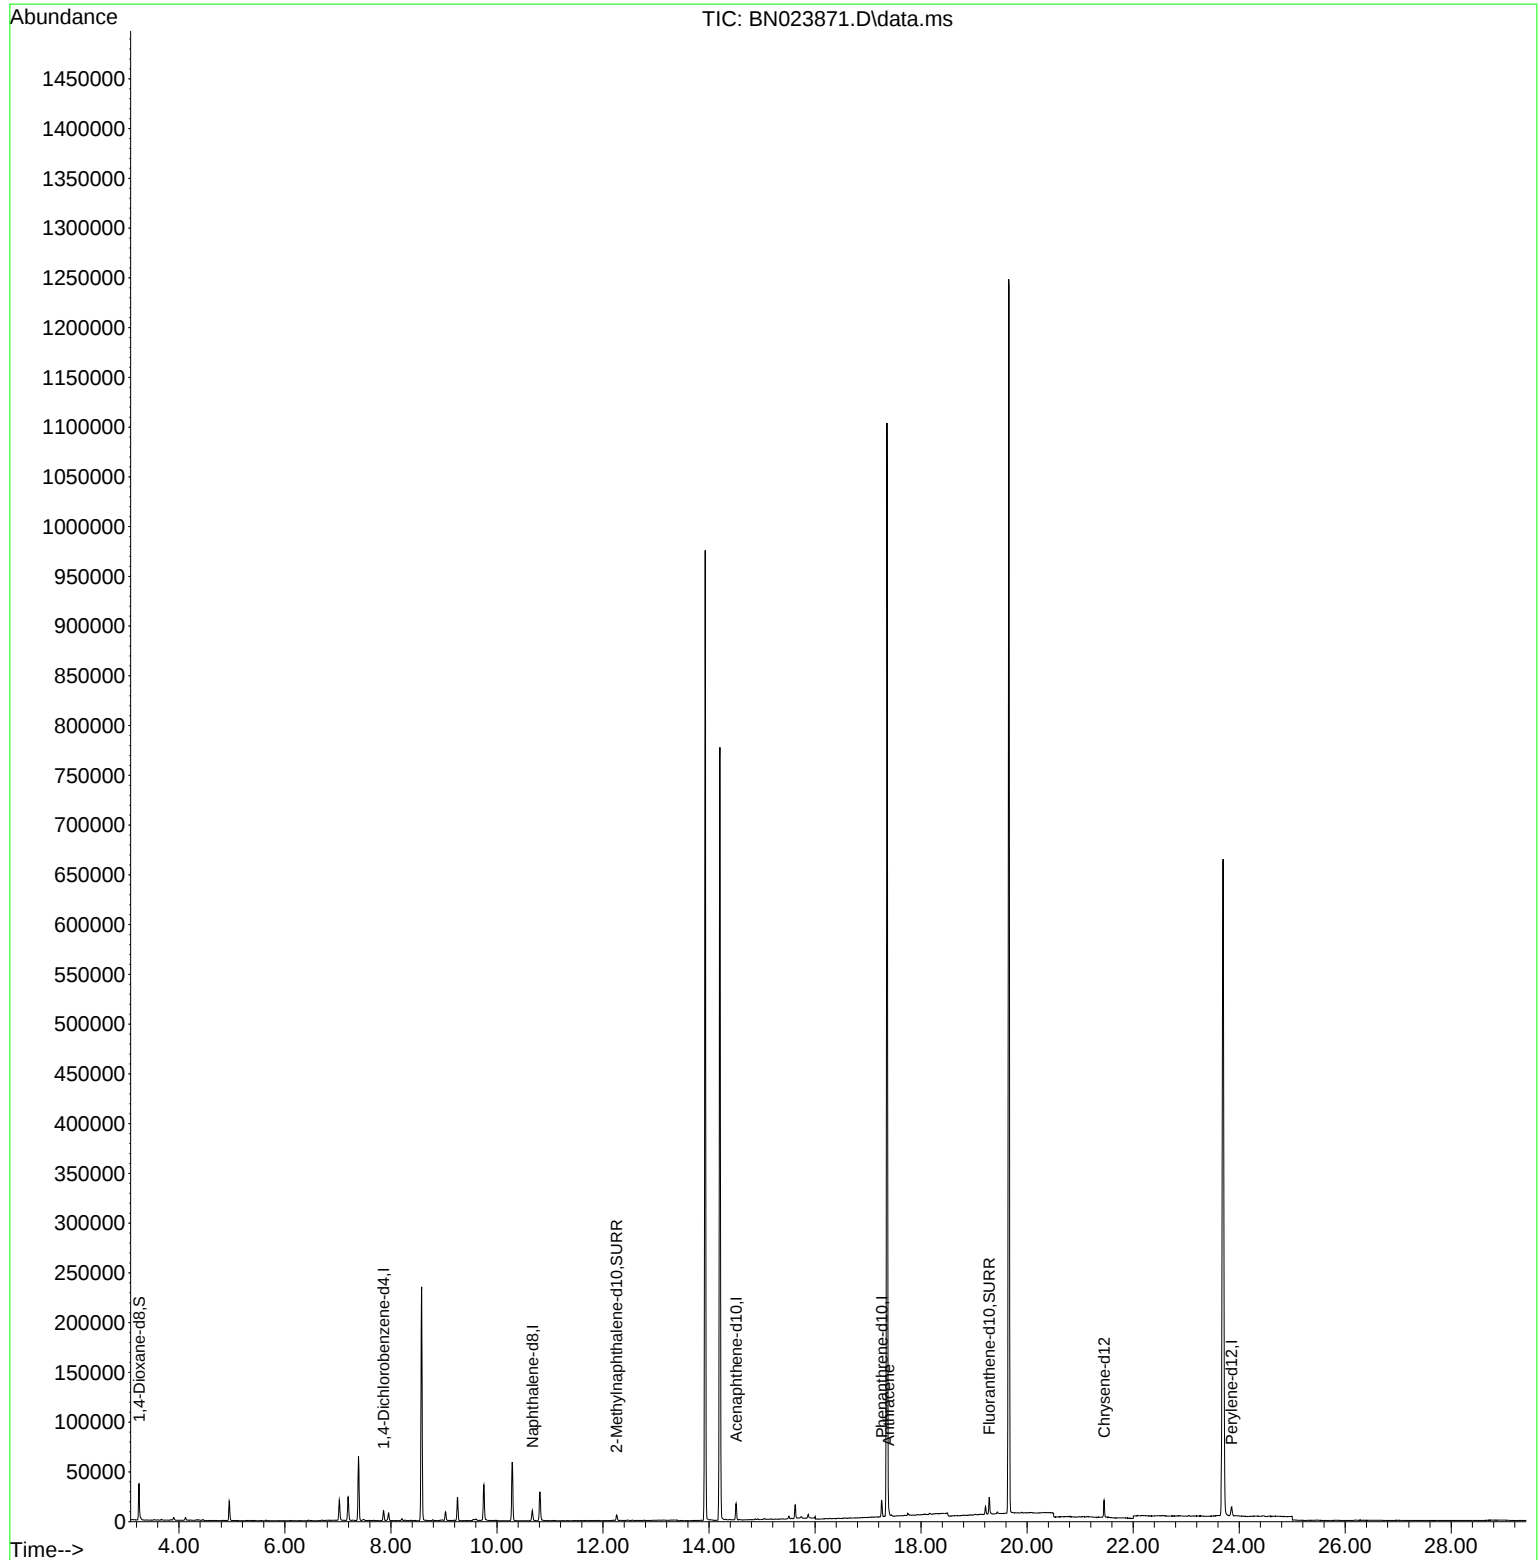

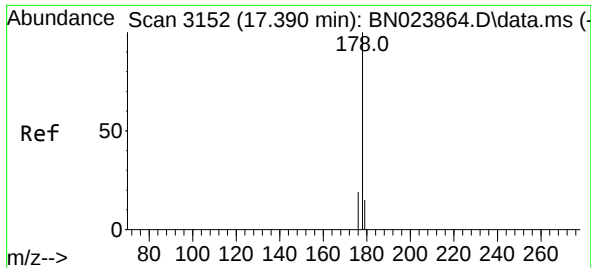

#16
 Anthracene
 Concen: 0.066 ng/ul
 RT: 17.390 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN023871.D
 Acq: 31 Jan 2023 21:07

Instrument :
 BNA_N
 ClientSampleId :
 EX9H3

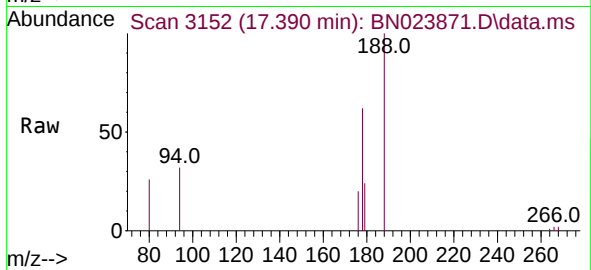

Tgt Ion:178 Resp: 3238
 Ion Ratio Lower Upper
 178 100
 179 38.5 13.4 20.0#
 176 32.9 15.4 23.2#

