

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
 Data File : BN023872.D
 Acq On : 31 Jan 2023 21:44
 Operator : CG/JU
 Sample : 01277-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9G8

Quant Time: Feb 01 01:07:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 01 01:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	5227	0.400	ng/ul	0.00
4) Naphthalene-d8	10.665	136	14815	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.510	164	9552	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.258	188	22283	0.400	ng/ul	0.00
17) Chrysene-d12	21.446	240	19818	0.400	ng/ul	0.00
23) Perylene-d12	23.837	264	16121	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.243	96	22905	4.088	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.260	152	7048	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.284	212	19933	0.374	ng/ul	0.00
Target Compounds						
16) Anthracene	17.393	178	1570	0.028	ng/ul#	Qvalue 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
Data File : BN023872.D
Acq On : 31 Jan 2023 21:44
Operator : CG/JU
Sample : 01277-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9G8


Quant Time: Feb 01 01:07:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:00:14 2023
Response via : Initial Calibration

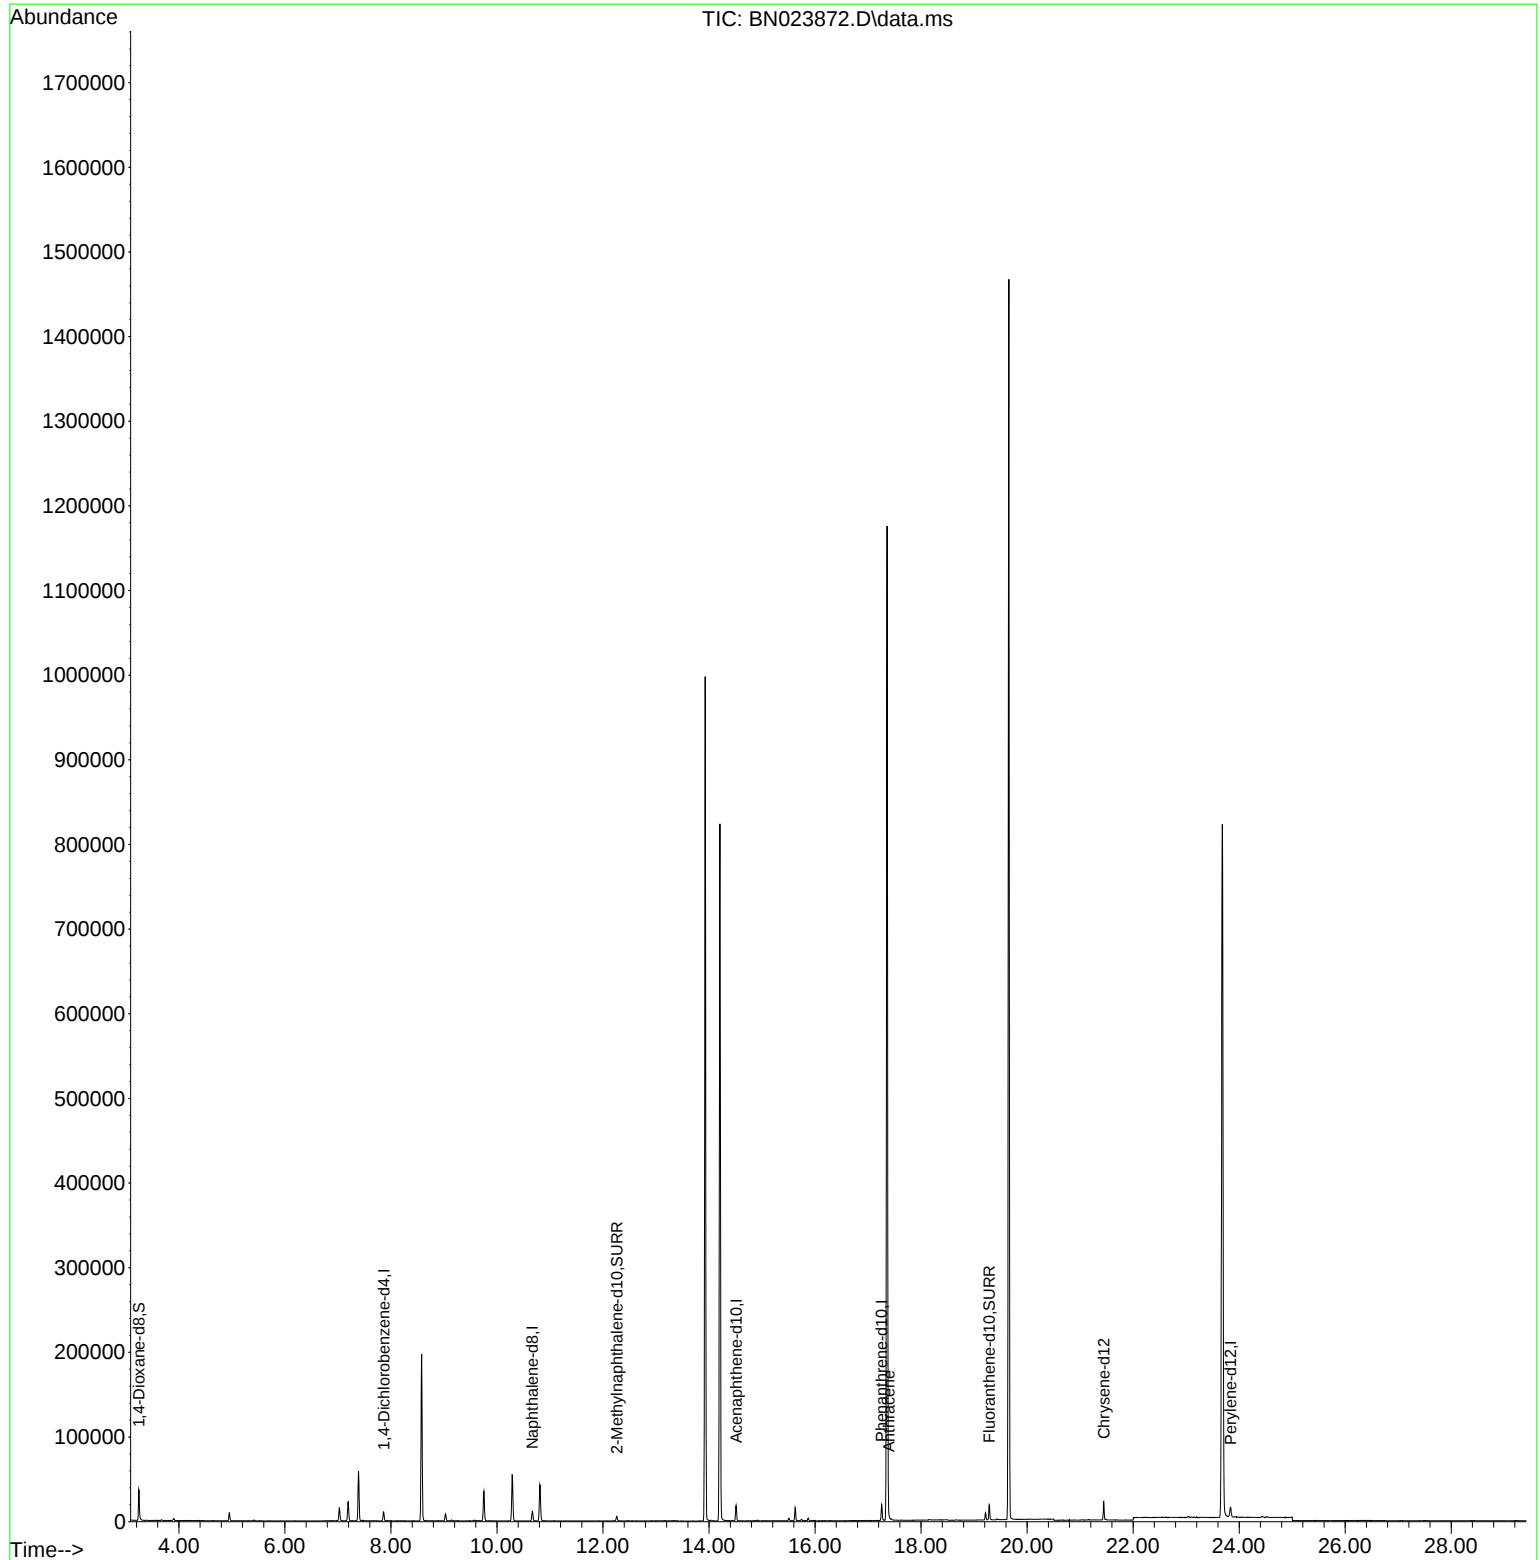

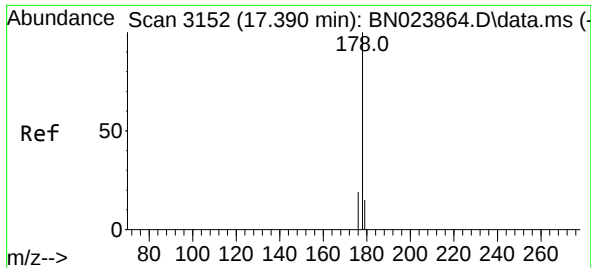

#16
 Anthracene
 Concen: 0.028 ng/ul
 RT: 17.393 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: BN023872.D
 Acq: 31 Jan 2023 21:44

Instrument :
 BNA_N
 ClientSampleId :
 EX9G8

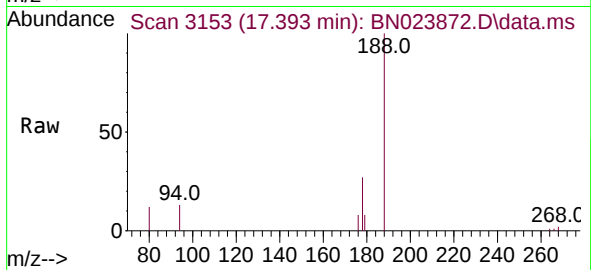

Tgt Ion:178 Resp: 1570
 Ion Ratio Lower Upper
 178 100
 179 30.7 13.4 20.0#
 176 27.9 15.4 23.2#

