

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
 Data File : BN023873.D
 Acq On : 31 Jan 2023 22:20
 Operator : CG/JU
 Sample : 01277-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9G9

Quant Time: Feb 01 01:08:11 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 01 01:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	4512	0.400	ng/ul	0.00
4) Naphthalene-d8	10.667	136	12941	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.512	164	8350	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.256	188	19515	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.441	240	17614	0.400	ng/ul	-0.01
23) Perylene-d12	23.824	264	14430	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.243	96	20875	4.316	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.256	152	6816	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.286	212	19885	0.420	ng/ul	0.00
Target Compounds						
16) Anthracene	17.391	178	1446	0.030	ng/ul#	Qvalue 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
Data File : BN023873.D
Acq On : 31 Jan 2023 22:20
Operator : CG/JU
Sample : 01277-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9G9


Quant Time: Feb 01 01:08:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:00:14 2023
Response via : Initial Calibration

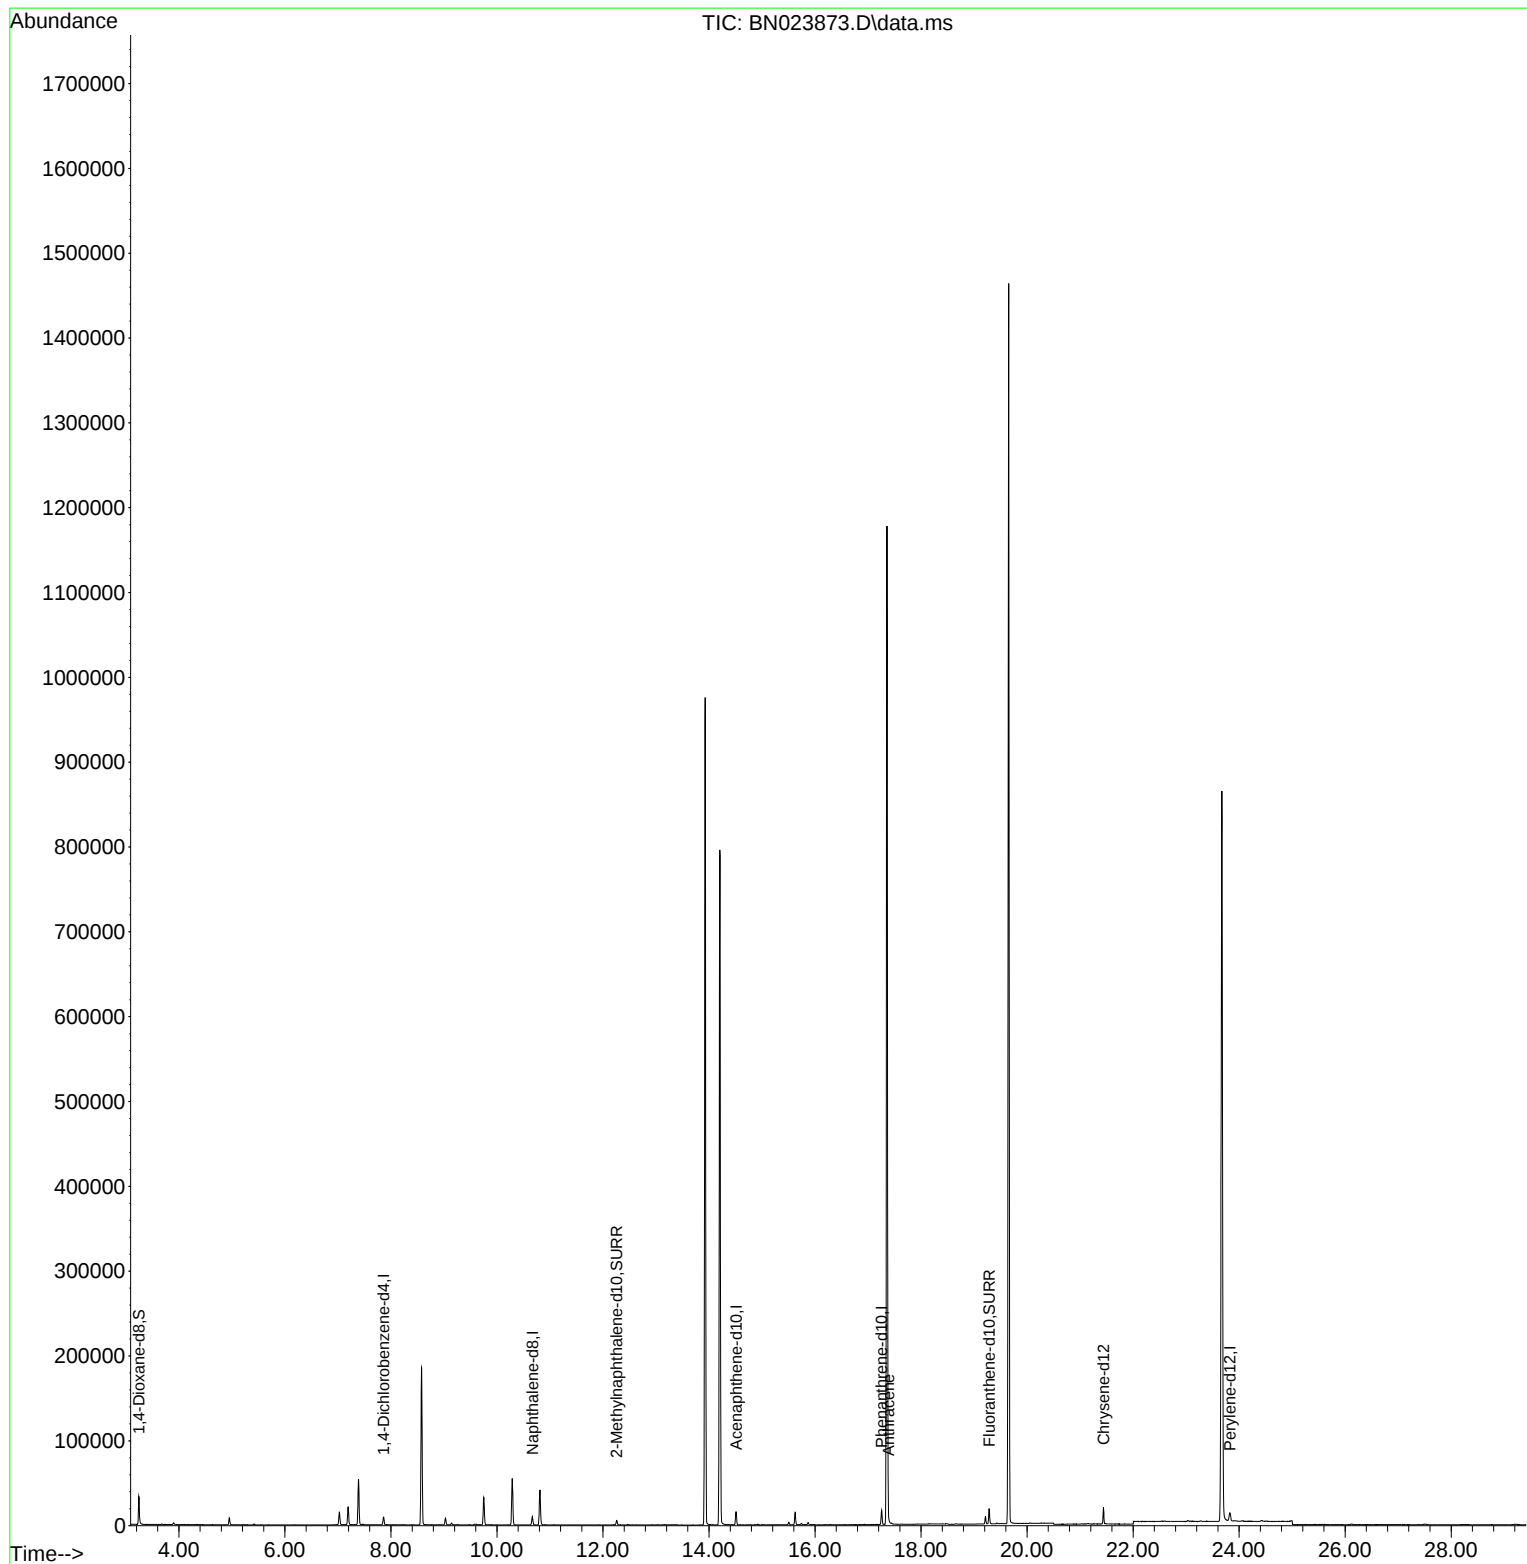

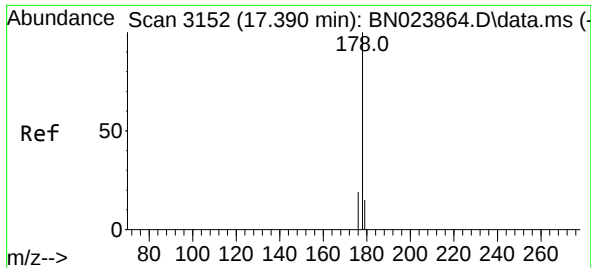

#16
 Anthracene
 Concen: 0.030 ng/ul
 RT: 17.391 min Scan# 31
 Delta R.T. 0.001 min
 Lab File: BN023873.D
 Acq: 31 Jan 2023 22:20

Instrument :
 BNA_N
 ClientSampleId :
 EX9G9

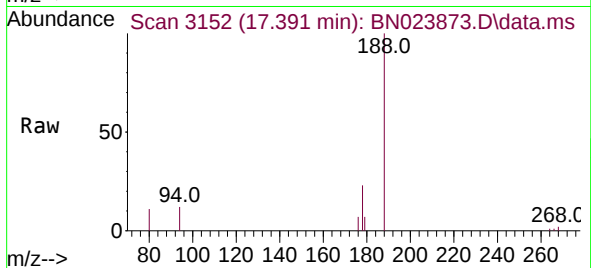

Tgt Ion:	178	Resp:	1446
Ion	Ratio	Lower	Upper
178	100		
179	32.6	13.4	20.0#
176	30.2	15.4	23.2#

