

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
 Data File : BN023876.D
 Acq On : 01 Feb 2023 00:11
 Operator : CG/JU
 Sample : 01278-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9H3

Quant Time: Feb 01 01:10:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 01 01:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	5721	0.400	ng/ul	0.00
4) Naphthalene-d8	10.665	136	16260	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.510	164	10595	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.258	188	23980	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.447	240	19605	0.400	ng/ul	# 0.00
23) Perylene-d12	23.835	264	16127	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.243	96	24278	3.959	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.260	152	8097	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.289	212	20451	0.388	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	690	0.106	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
Data File : BN023876.D
Acq On : 01 Feb 2023 00:11
Operator : CG/JU
Sample : 01278-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9H3


Quant Time: Feb 01 01:10:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:00:14 2023
Response via : Initial Calibration

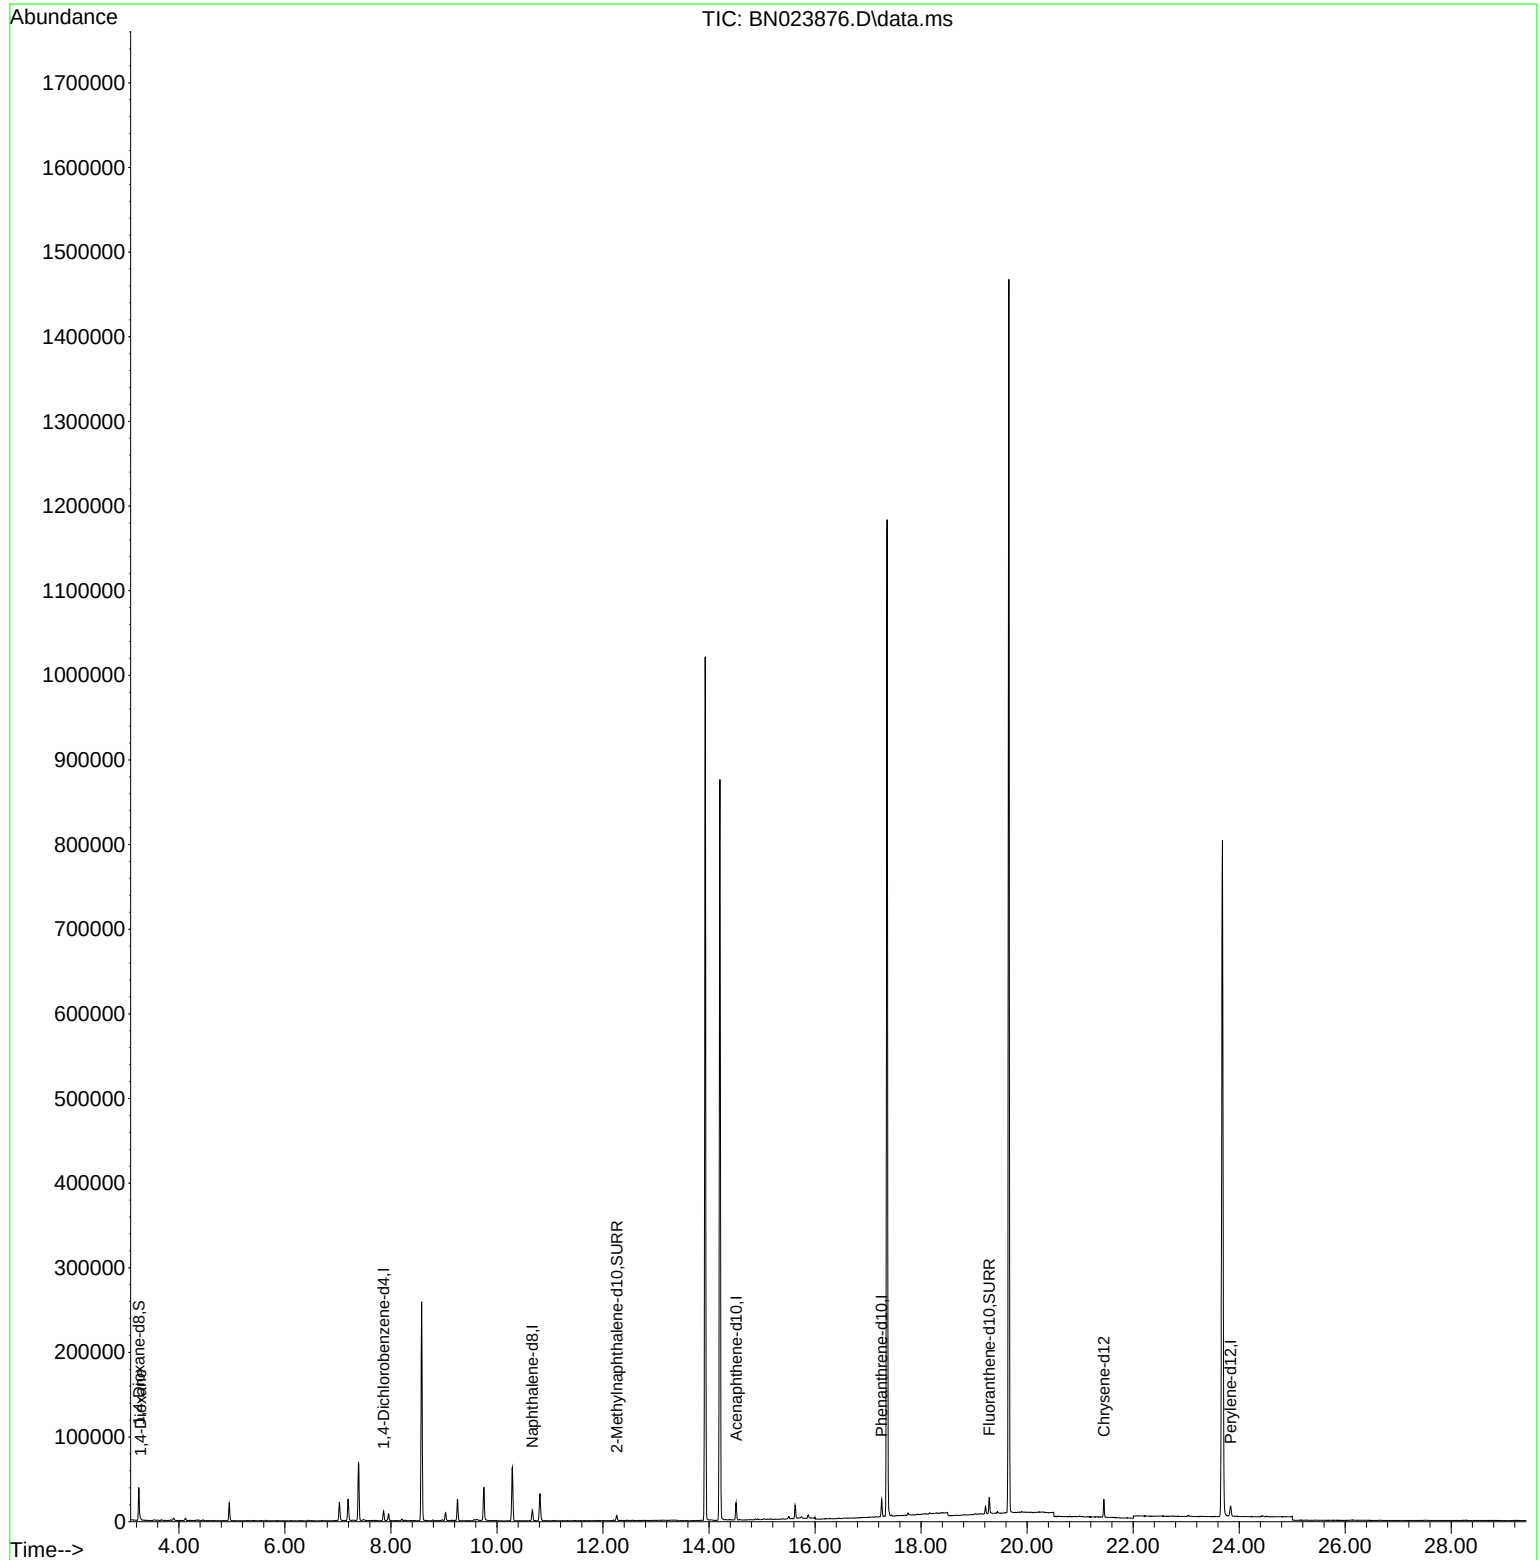

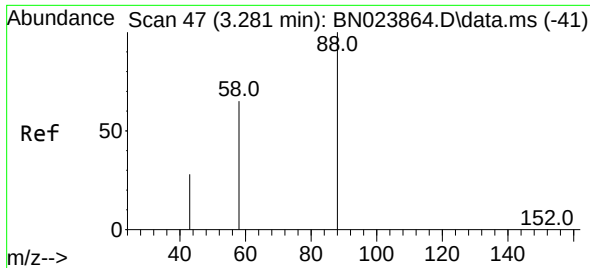

#2
 1,4-Dioxane
 Concen: 0.106 ng/ul
 RT: 3.281 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN023876.D
 Acq: 01 Feb 2023 00:11

Instrument :
 BNA_N
 ClientSampleId :
 EX9H3

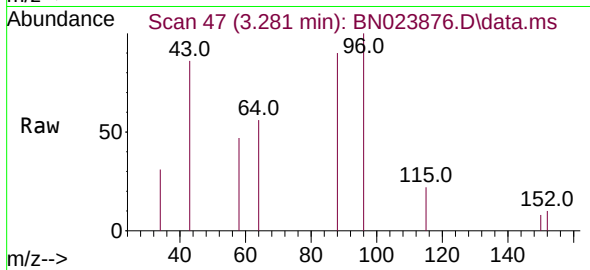

Tgt Ion: 88	Resp: 690
Ion Ratio	Lower Upper
88 100	
43 94.9	41.9 62.9#
58 51.6	45.6 68.4

