

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
 Data File : BN023877.D
 Acq On : 01 Feb 2023 00:48
 Operator : CG/JU
 Sample : 01278-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EX9G8

Quant Time: Feb 01 01:19:56 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 01 01:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	4483	0.400	ng/ul	0.00
4) Naphthalene-d8	10.667	136	12641	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.507	164	8203	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.256	188	19309	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.450	240	18683	0.400	ng/ul	# 0.00
23) Perylene-d12	23.856	264	16111	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.243	96	19182	3.992	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.256	152	6603	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.286	212	19376	0.386	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.281	88	214	0.042	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013123\
Data File : BN023877.D
Acq On : 01 Feb 2023 00:48
Operator : CG/JU
Sample : 01278-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EX9G8


Quant Time: Feb 01 01:19:56 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:00:14 2023
Response via : Initial Calibration

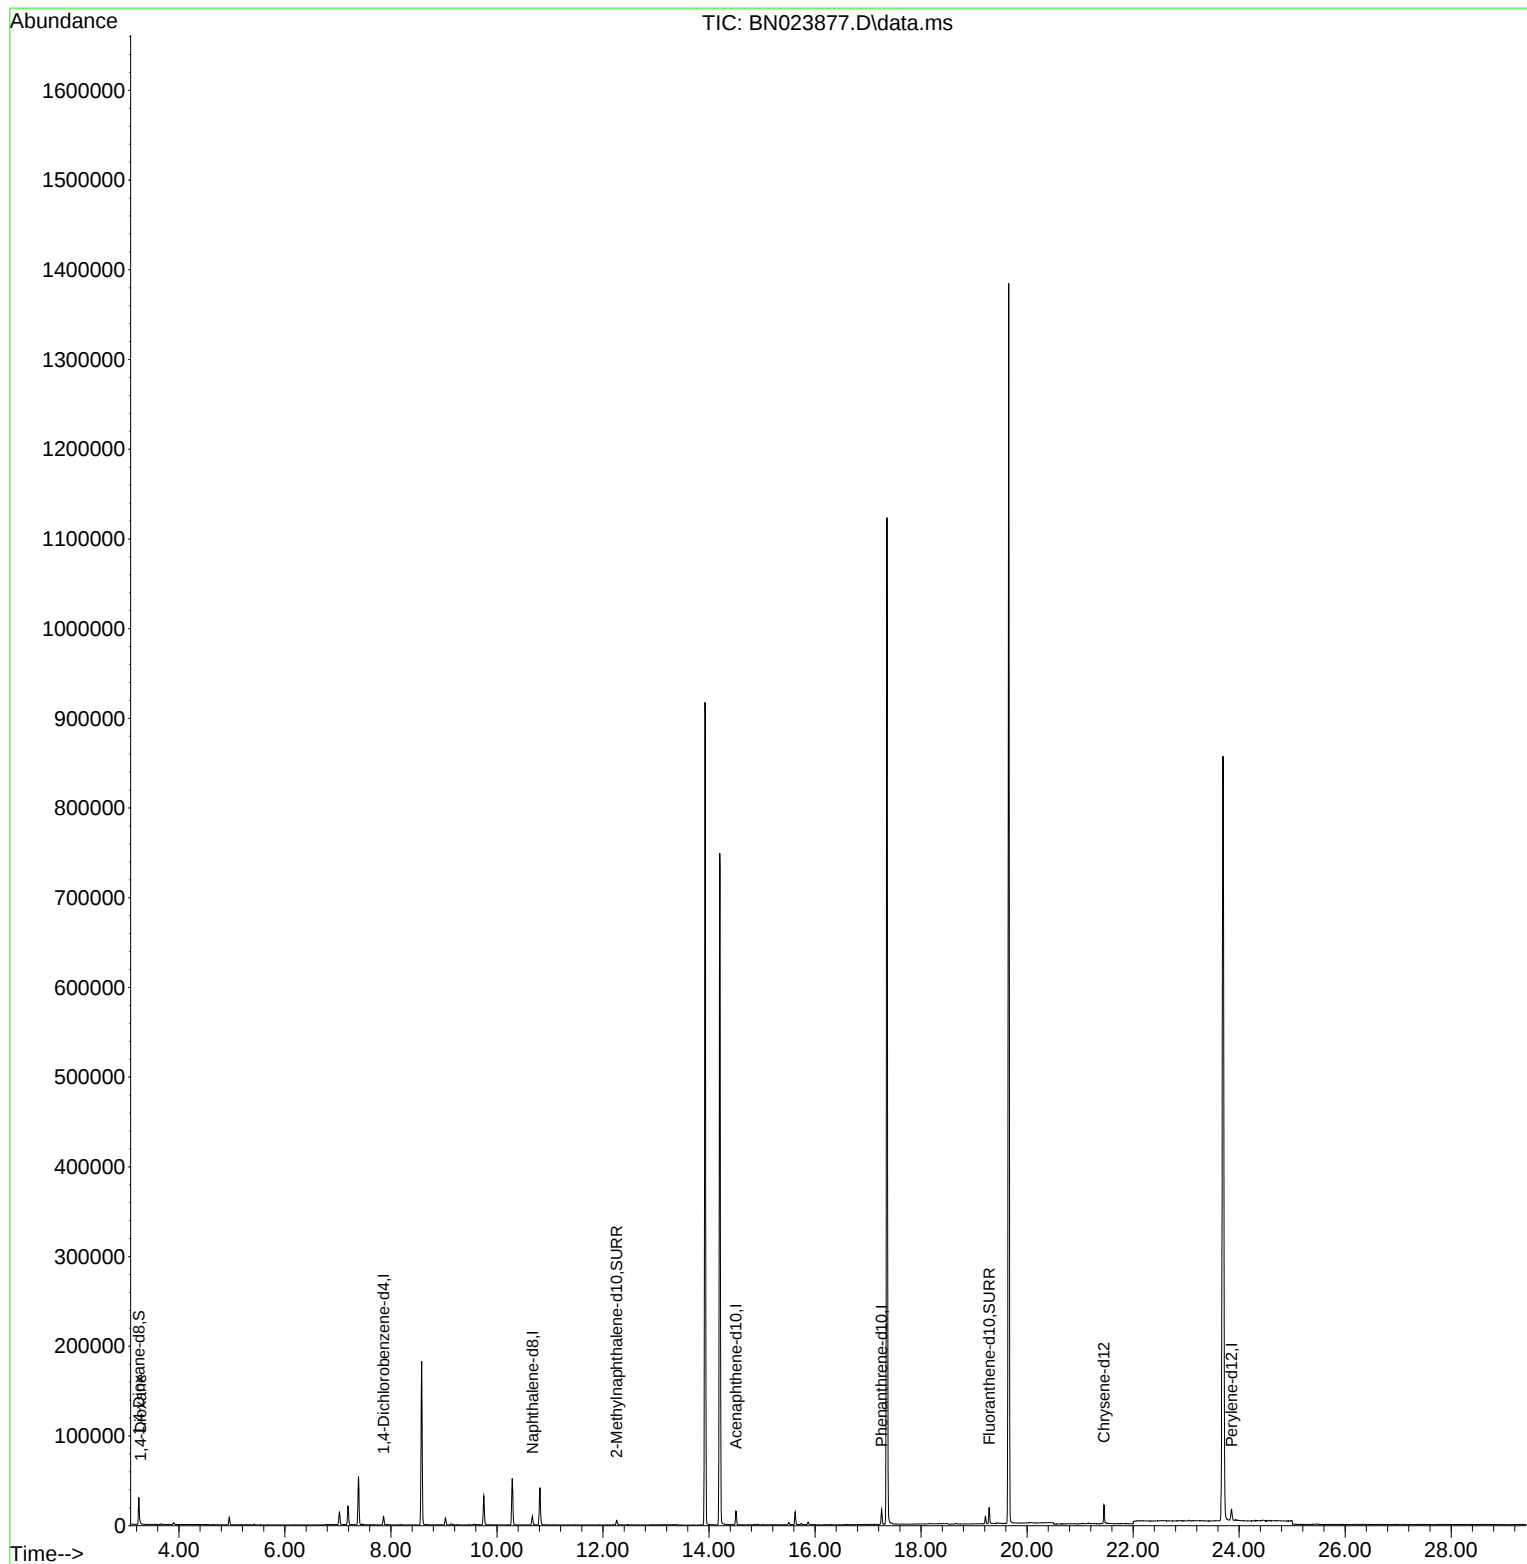

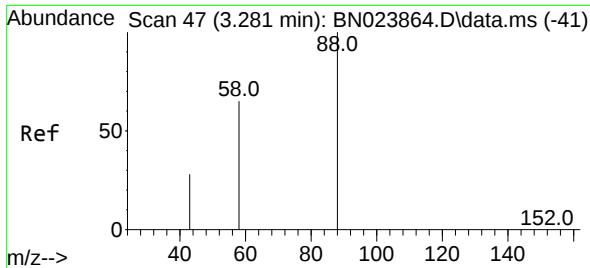

#2
 1,4-Dioxane
 Concen: 0.042 ng/ul
 RT: 3.281 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN023877.D
 Acq: 01 Feb 2023 00:48

Instrument :
 BNA_N
 ClientSampleId :
 EX9G8

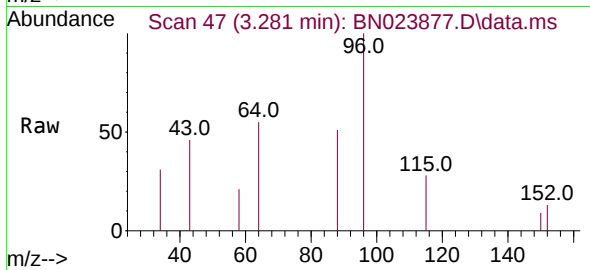

Tgt Ion: 88	Resp: 214
Ion Ratio	Lower Upper
88	100
43	90.3 41.9 62.9#
58	42.0 45.6 68.4#

