
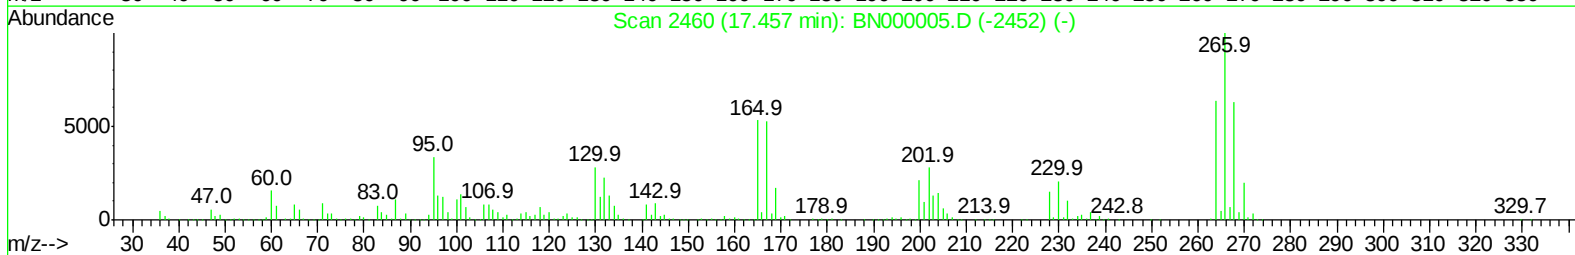
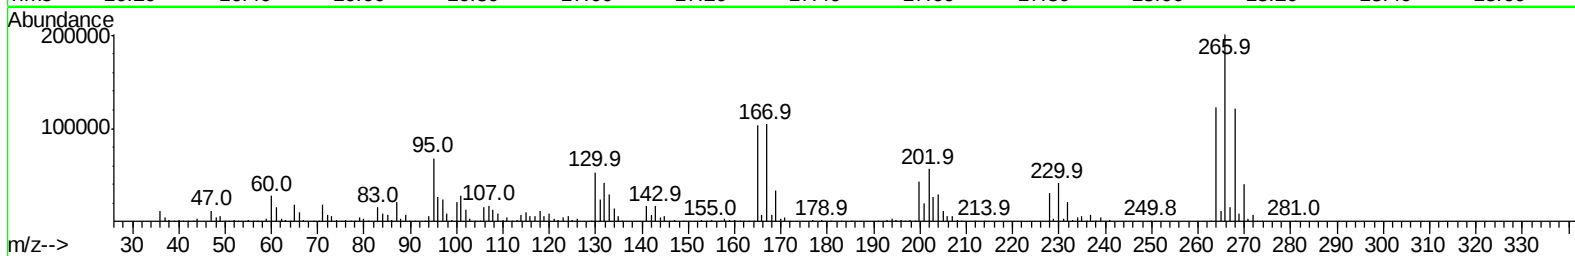


Data Path : U:\HPCHEM1\BNA N\DATA\BN020618\
Data File : BN000021.D
Acq On : 06 Feb 2018 08:28
Operator :
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:49:08 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 15:24:10 2018
Response via : Initial Calibration

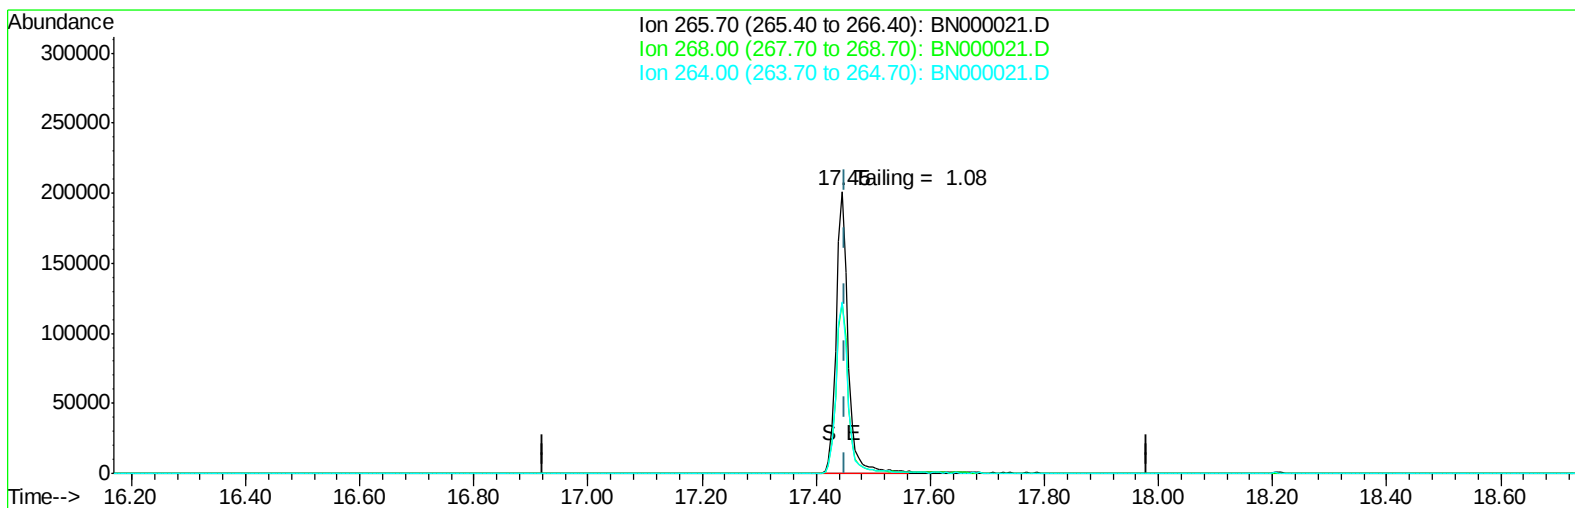

TIC: BN000021.D

(69) Pentachlorophenol (C)




17.445min (-0.006) 123164.64ng

response 291852

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.27
264.00	62.00	60.84
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA N\DATA\BN020618\
 Data File : BN000021.D
 Acq On : 06 Feb 2018 08:28
 Operator :
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:49:08 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 15:24:10 2018
 Response via : Initial Calibration

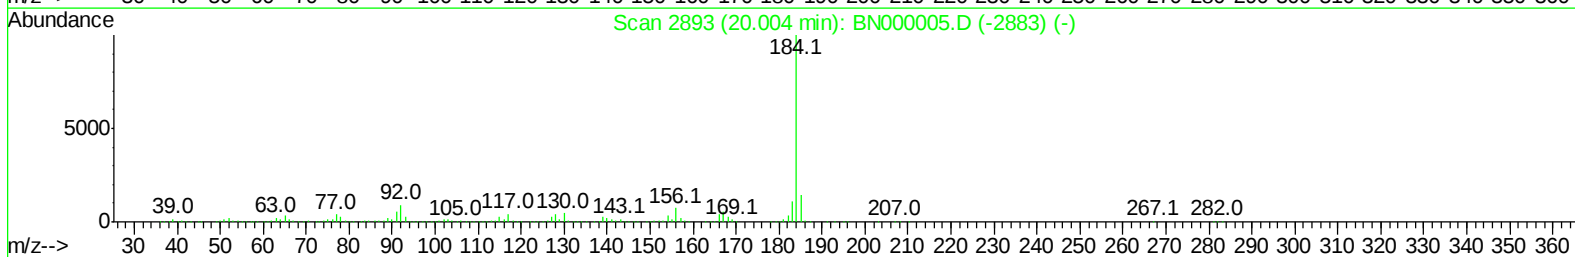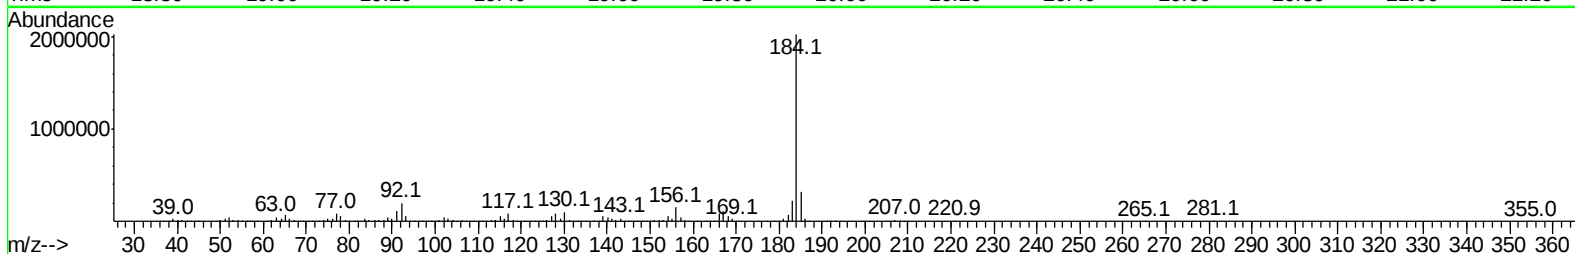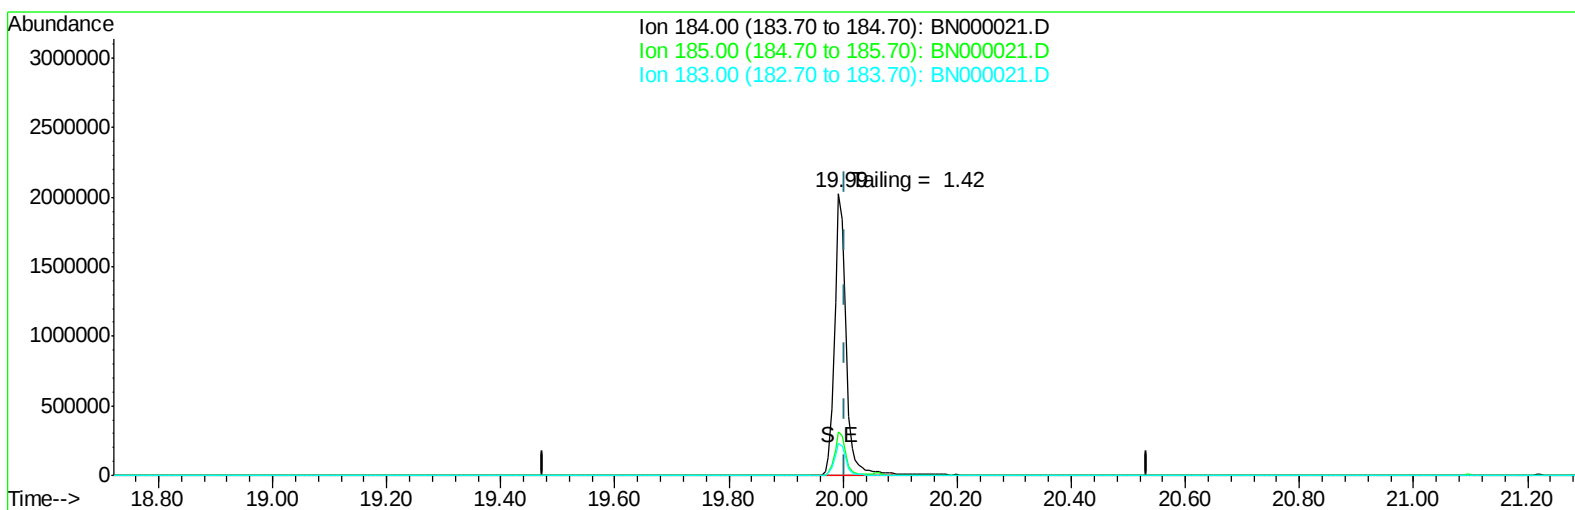

TIC: BN000021.D

(76) Benzidine

19.992min (-0.012) 25013.48ng

response 2784639

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.51
183.00	13.30	11.32
0.00	0.00	0.00