

Data Path : Z:\HPCHEM1\BNA N\DATA\BN020618\
 Data File : BN000024.D
 Acq On : 06 Feb 2018 10:10
 Operator :
 Sample : PB106300BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB106300BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.946	495	503	520	rBV	5304170	9021964	32.68%	7.141%
2	7.593	775	783	802	rBV	6064359	10135170	36.71%	8.022%
3	7.993	843	851	865	rBV	5855943	9780487	35.43%	7.741%
4	8.475	923	933	940	rBV	1100587	1827591	6.62%	1.447%
5	8.805	981	989	998	rVB	4206585	7048226	25.53%	5.579%
6	9.652	1124	1133	1147	rBV	3274460	5321994	19.28%	4.212%
7	11.316	1407	1416	1424	rBV	1714616	2923669	10.59%	2.314%
8	13.716	1817	1824	1833	rBV	10705106	15560907	56.37%	12.317%
9	15.081	2049	2056	2067	rBV2	2804750	4232528	15.33%	3.350%
10	16.551	2299	2306	2327	rBV	6999210	10068656	36.47%	7.969%
11	17.804	2512	2519	2528	rBV	4296858	5842132	21.16%	4.624%
12	20.369	2949	2955	2967	rBV	21166332	27605968	100.00%	21.850%
13	21.927	3214	3220	3229	rBV	6044707	8107829	29.37%	6.417%
14	24.421	3636	3644	3661	rBV	4469469	8864439	32.11%	7.016%


Sum of corrected areas: 126341560

Data Path : Z:\HPCHEM1\BNA N\DATA\BN020618\
Data File : BN000024.D
Acq On : 06 Feb 2018 10:10
Operator :
Sample : PB106300BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB106300BL

Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

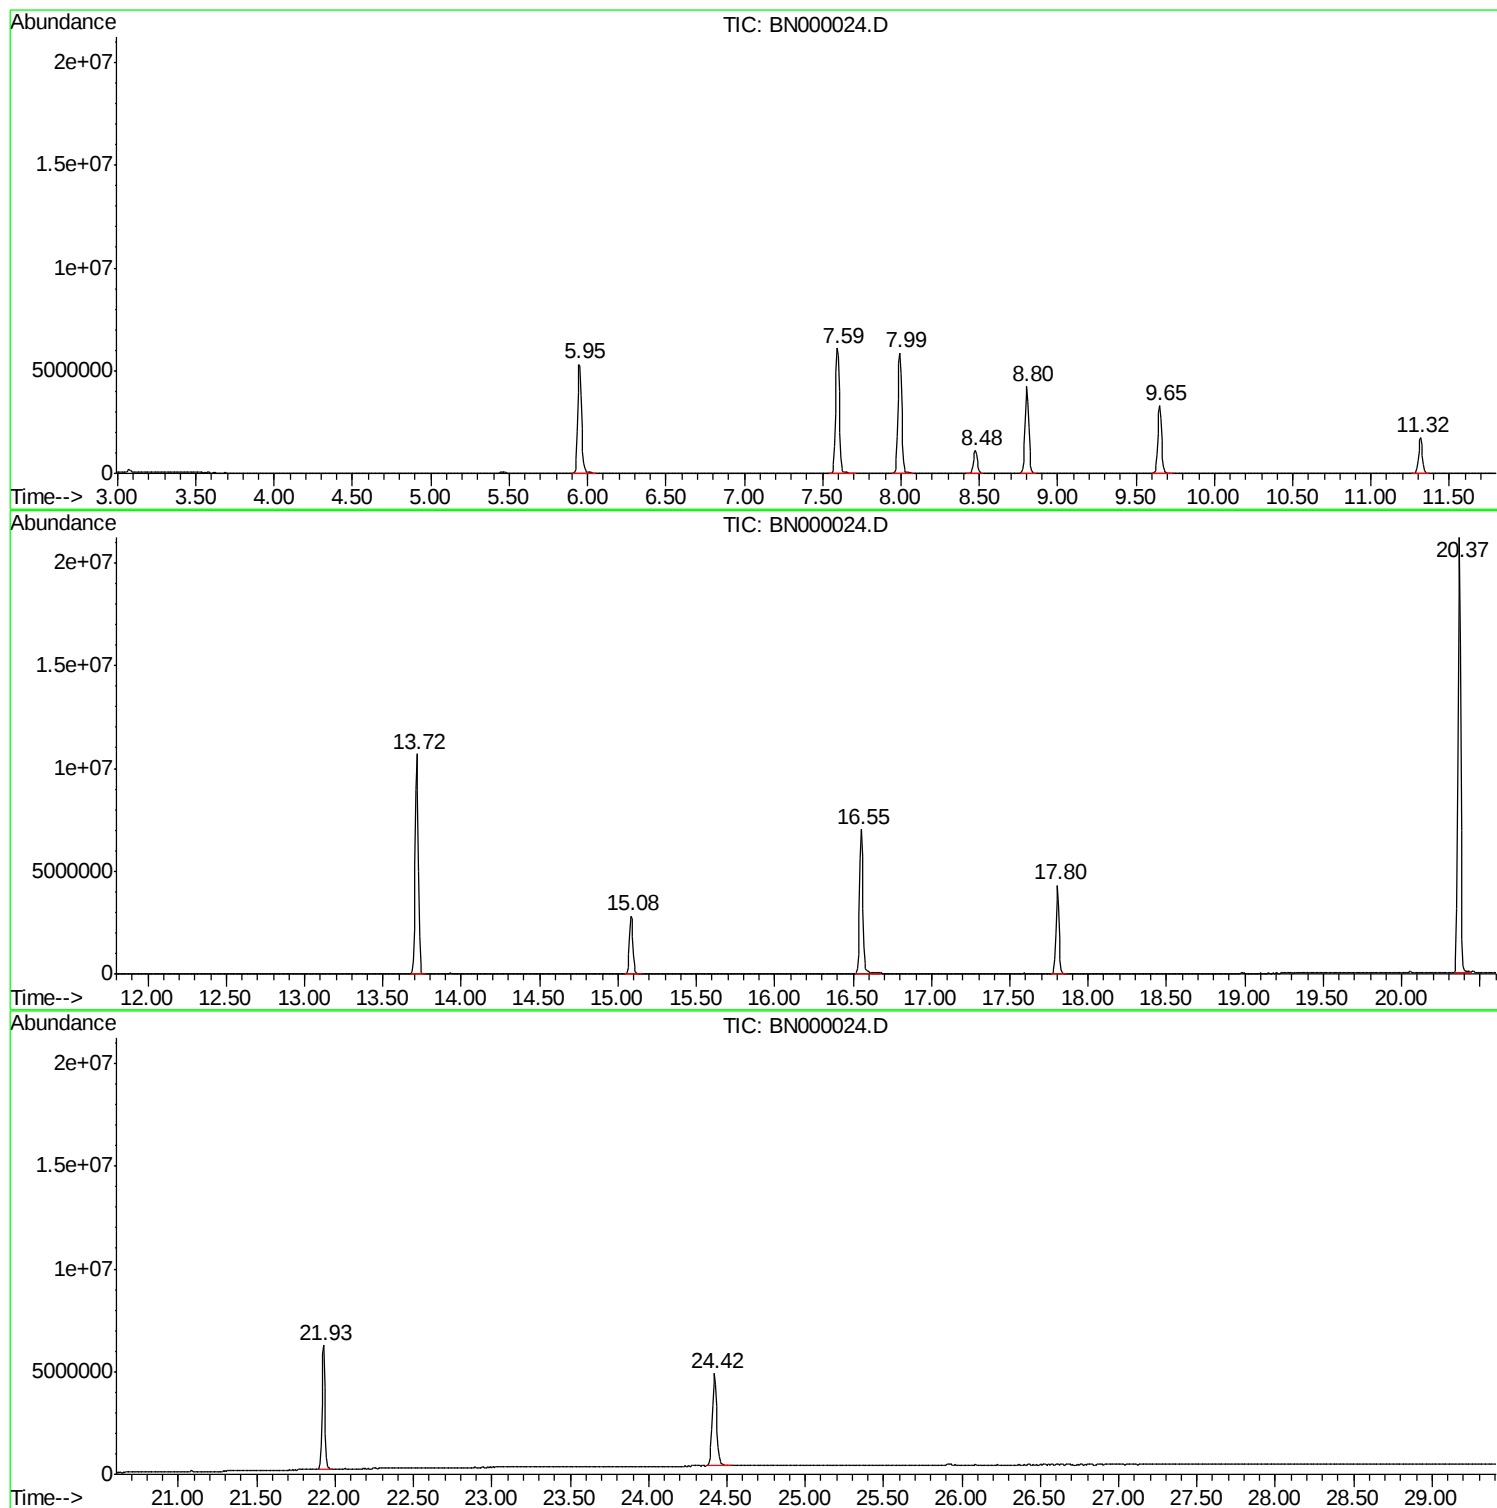

Data Path : Z:\HPCHEM1\BNA N\DATA\BN020618\
Data File : BN000024.D
Acq On : 06 Feb 2018 10:10
Operator :
Sample : PB106300BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB106300BL










Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.99 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.99	107.03 ng	9780490	1,4-Dichlorobenzene-d4	8.48

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

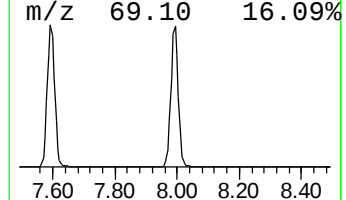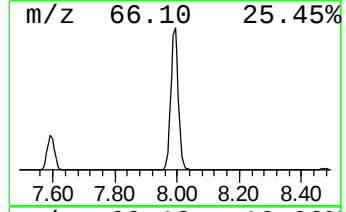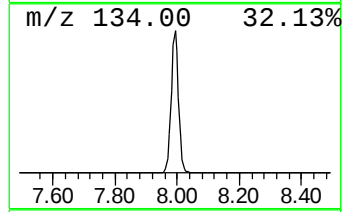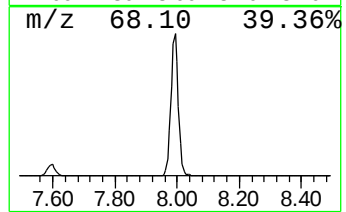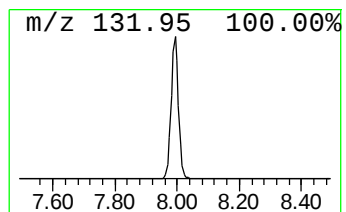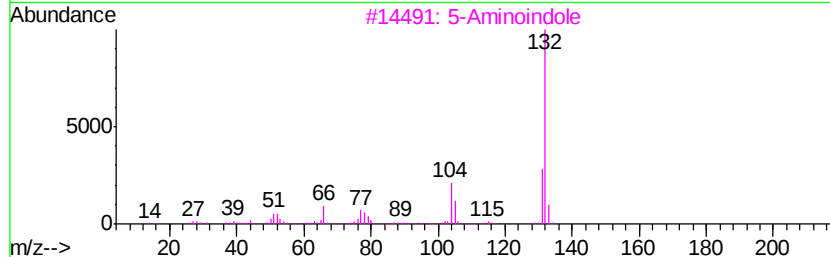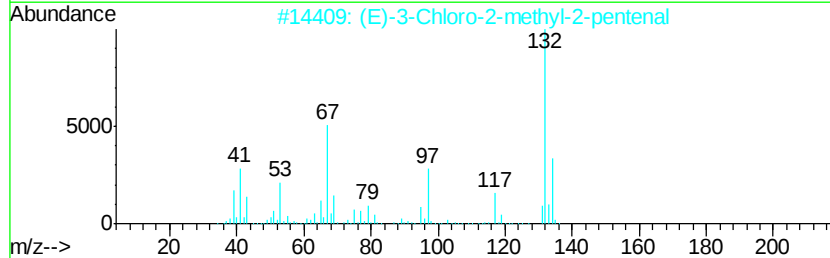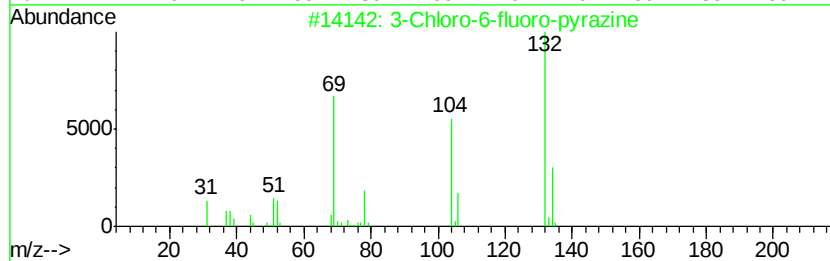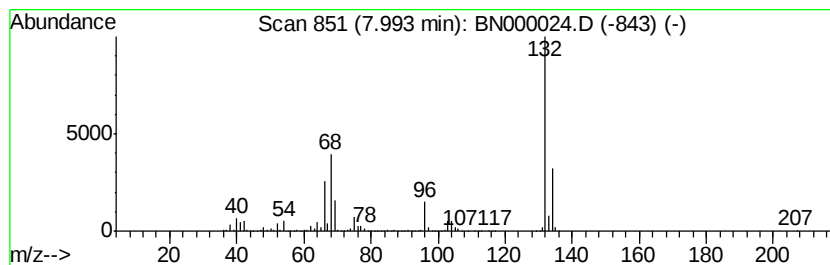

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN020618\
Data File : BN000024.D
Acq On : 06 Feb 2018 10:10
Operator :
Sample : PB106300BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB106300BL

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.99	7.99	107.0	ng	9780490	1	8.48	1827590	20.0