

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020620\
 Data File : BN009676.D
 Acq On : 08 Feb 2020 09:33
 Operator : CG/JU
 Sample : L1401-20
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6X8

Quant Time: Feb 10 03:42:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 15:21:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	152555	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	631816	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	384276	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.82	188	816378	20.00	ng/ul	0.00
77) Chrysene-d12	21.03	240	784076	20.00	ng/ul	-0.01
85) Perylene-d12	23.15	264	783637	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	21763	5.85	ng/uL	0.00
5) Phenol-d5	6.63	99	418536	31.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	289057	32.34	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	323812	33.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.14	113	336170	31.73	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	161324	34.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	185947	35.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	319620	32.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	449092	42.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.49	166	981183	34.98	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	1199448	35.39	ng/ul	0.00
51) 4-Nitrophenol-d4	14.30	143	163133	30.79	ng/ul	0.00
57) Fluorene-d10	15.07	176	855993	34.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	140387	27.53	ng/ul	0.00
70) Anthracene-d10	16.92	188	1313416	35.41	ng/ul	0.00
78) Pyrene-d10	19.23	212	1425800	34.59	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	1397244	36.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.54	163	58588	1.968	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020620\
Data File : BN009676.D
Acq On : 08 Feb 2020 09:33
Operator : CG/JU
Sample : L1401-20
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6X8

Quant Time: Feb 10 03:42:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 15:21:46 2020
Response via : Initial Calibration

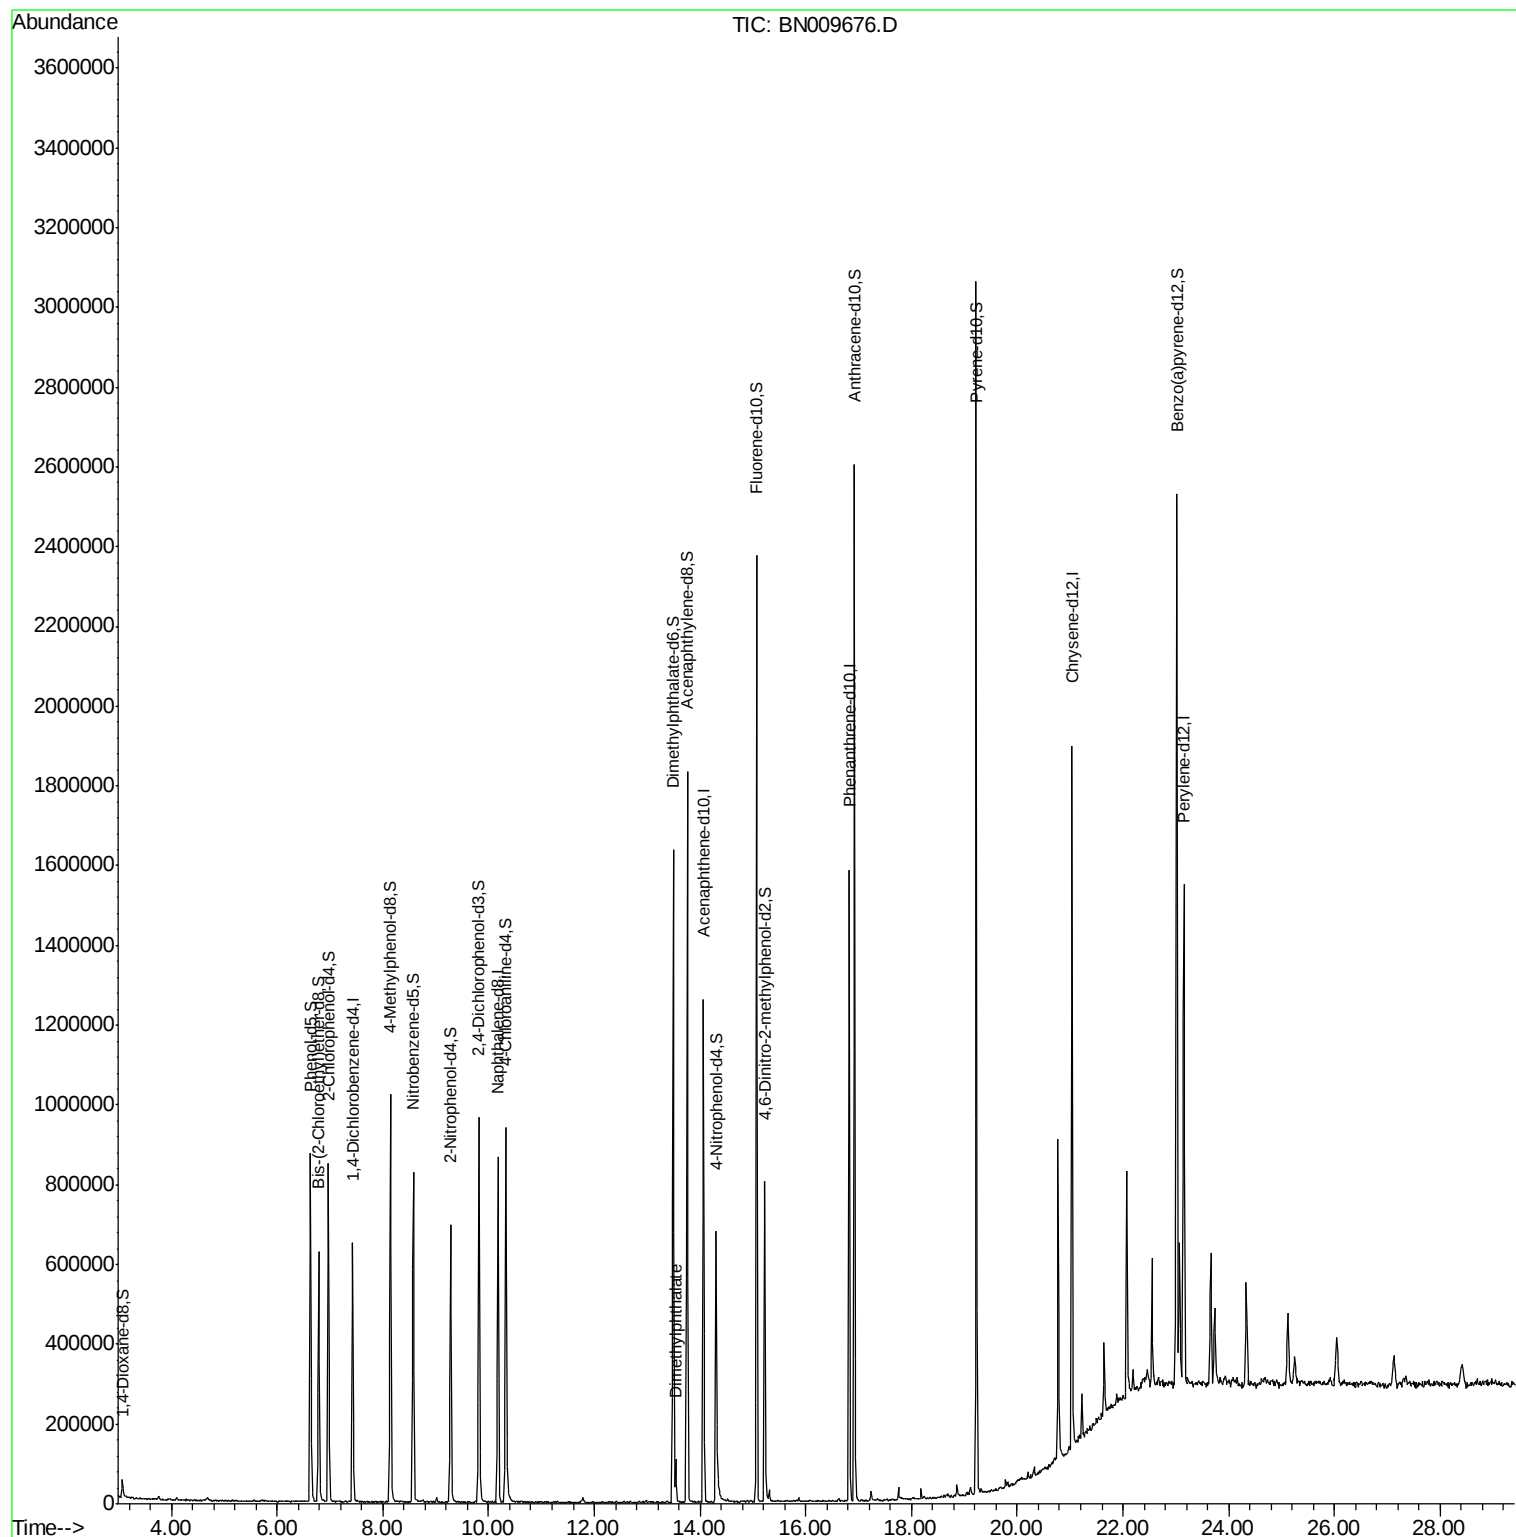

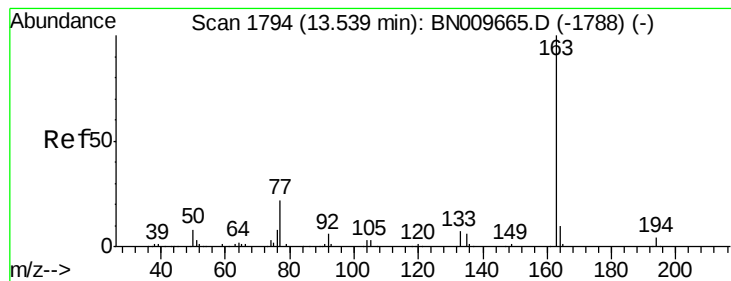

#44
 Dimethylphthalate
 Concen: 1.968 ng/ul
 RT: 13.54 min Scan# 1794
 Delta R.T. -0.01 min
 Lab File: BN009676.D
 Acq: 08 Feb 2020 09:33

Instrument :
 BNA_N
 ClientSampleId :
 CB6X8

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.5	5.3
164	9.7	8.0	12.0

