

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020620\
 Data File : BN009626.D
 Acq On : 07 Feb 2020 01:11
 Operator : CG/JU
 Sample : TESTBL-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.075	12	15	22	rBV2	20112	27811	0.77%	0.074%
2	3.405	68	71	74	rBV3	3332	3616	0.10%	0.010%
3	3.764	128	132	135	rVB4	5669	8233	0.23%	0.022%
4	3.946	161	163	169	rVB4	2568	4651	0.13%	0.012%
5	4.187	200	204	208	rBV2	6319	6341	0.18%	0.017%
6	4.599	271	274	277	rBV4	3230	4451	0.12%	0.012%
7	6.634	613	620	631	rBV	441739	709555	19.66%	1.881%
8	6.793	641	647	660	rVB	587029	907035	25.13%	2.405%
9	6.975	672	678	689	rVB	757699	1170848	32.44%	3.104%
10	7.434	750	756	768	rVB	575870	890963	24.68%	2.362%
11	7.528	768	772	776	rBV4	3694	5970	0.17%	0.016%
12	8.146	869	877	886	rBV	748034	1169069	32.39%	3.100%
13	8.258	891	896	903	rBV2	20208	34841	0.97%	0.092%
14	8.575	940	950	962	rBV	813668	1310349	36.30%	3.474%
15	8.758	978	981	987	rVB4	9888	14179	0.39%	0.038%
16	9.022	1021	1026	1028	rBV3	3277	3626	0.10%	0.010%
17	9.087	1033	1037	1040	rBV4	3628	4506	0.12%	0.012%
18	9.152	1042	1048	1051	rVB5	3350	5429	0.15%	0.014%
19	9.287	1065	1071	1081	rBV	670120	1104386	30.60%	2.928%
20	9.822	1155	1162	1178	rBV	858855	1530971	42.42%	4.059%
21	10.187	1216	1224	1233	rVB	780914	1291874	35.79%	3.425%
22	10.340	1244	1250	1262	rBV2	90220	187382	5.19%	0.497%
23	10.422	1262	1264	1270	rVB5	4654	7319	0.20%	0.019%
24	10.781	1321	1325	1327	rBV3	3041	3877	0.11%	0.010%
25	10.840	1329	1335	1340	rBV3	3085	7194	0.20%	0.019%
26	11.646	1466	1472	1478	rVB5	4788	7953	0.22%	0.021%
27	11.787	1491	1496	1504	rVB3	9524	16571	0.46%	0.044%
28	12.910	1684	1687	1692	rVB3	4244	5364	0.15%	0.014%
29	13.498	1780	1787	1795	rBV	1529454	2160692	59.86%	5.729%
30	13.757	1824	1831	1843	rBV	1627521	2433026	67.41%	6.451%
31	14.010	1870	1874	1878	rBV5	3516	5319	0.15%	0.014%
32	14.075	1878	1885	1893	rBV	1078441	1646691	45.62%	4.366%
33	14.234	1909	1912	1918	rVB5	7760	11094	0.31%	0.029%
34	14.310	1918	1925	1948	rBV	271347	569729	15.78%	1.511%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020620\
 Data File : BN009626.D
 Acq On : 07 Feb 2020 01:11
 Operator : CG/JU
 Sample : TESTBL-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Title : SVOA CALIBRATION

35	14.534	1959	1963	1971	rBV2	36117	51133	1.42%	0.136%
36	14.928	2024	2030	2033	rBV3	7117	9870	0.27%	0.026%
37	14.969	2033	2037	2039	rBV3	6969	6438	0.18%	0.017%
38	15.075	2048	2055	2066	rBV	2309776	3179828	88.10%	8.431%
39	15.222	2074	2080	2092	rBV	774903	1123257	31.12%	2.978%
40	15.316	2092	2096	2102	rVB	26889	37152	1.03%	0.099%
41	15.528	2130	2132	2136	rBV3	4073	4833	0.13%	0.013%
42	15.775	2170	2174	2178	rBV4	4615	7275	0.20%	0.019%
43	15.828	2181	2183	2187	rBV4	3479	5638	0.16%	0.015%
44	15.869	2187	2190	2192	rVB2	6126	7232	0.20%	0.019%
45	16.269	2253	2258	2263	rBV4	13819	18619	0.52%	0.049%
46	16.616	2314	2317	2323	rVB4	8207	13207	0.37%	0.035%
47	16.828	2347	2353	2359	rBV	1362908	1852327	51.32%	4.911%
48	16.928	2364	2370	2381	rVB	2051247	2888778	80.03%	7.659%
49	17.139	2399	2406	2412	rVB2	22136	37725	1.05%	0.100%
50	17.751	2506	2510	2516	rBV6	26223	38787	1.07%	0.103%
51	17.804	2516	2519	2525	rVB5	10211	19578	0.54%	0.052%
52	17.904	2532	2536	2540	rBV4	4399	6743	0.19%	0.018%
53	18.057	2557	2562	2564	rBV4	6529	11904	0.33%	0.032%
54	18.251	2592	2595	2600	rVB5	5194	7287	0.20%	0.019%
55	18.298	2600	2603	2605	rBV3	9580	9849	0.27%	0.026%
56	18.457	2628	2630	2633	rBV4	3896	4425	0.12%	0.012%
57	18.698	2666	2671	2675	rBV3	18275	26133	0.72%	0.069%
58	18.869	2693	2700	2706	rBV	31971	47645	1.32%	0.126%
59	19.045	2728	2730	2735	rBV4	11830	15069	0.42%	0.040%
60	19.116	2739	2742	2746	rVB2	19296	25116	0.70%	0.067%
61	19.233	2756	2762	2769	rBV	2755151	3609424	100.00%	9.570%
62	19.286	2769	2771	2773	rVB3	12440	9644	0.27%	0.026%
63	19.363	2782	2784	2789	rVB6	7713	9583	0.27%	0.025%
64	19.569	2817	2819	2821	rBV3	5415	4516	0.13%	0.012%
65	19.828	2859	2863	2865	rBV4	13555	17854	0.49%	0.047%
66	19.851	2865	2867	2870	rVV4	8503	9346	0.26%	0.025%
67	20.322	2945	2947	2951	rVB	24673	24620	0.68%	0.065%
68	20.792	3024	3027	3030	rVB3	47218	43877	1.22%	0.116%
69	21.039	3064	3069	3075	rBV	1646533	1991274	55.17%	5.280%
70	21.227	3098	3101	3106	rVB	83840	85509	2.37%	0.227%
71	21.645	3169	3172	3178	rBV	107934	122028	3.38%	0.324%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020620\
Data File : BN009626.D
Acq On : 07 Feb 2020 01:11
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL-01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Title : SVOA CALIBRATION

72	22.080	3243	3246	3251	rVB	144360	177230	4.91%	0.470%
73	22.551	3324	3326	3332	rVB2	126121	171126	4.74%	0.454%
74	23.021	3400	3406	3412	rBV	1694369	2741396	75.95%	7.269%
75	23.151	3422	3428	3439	rVB2	1095549	1971442	54.62%	5.227%


Sum of corrected areas: 37715632

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020620\
Data File : BN009626.D
Acq On : 07 Feb 2020 01:11
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

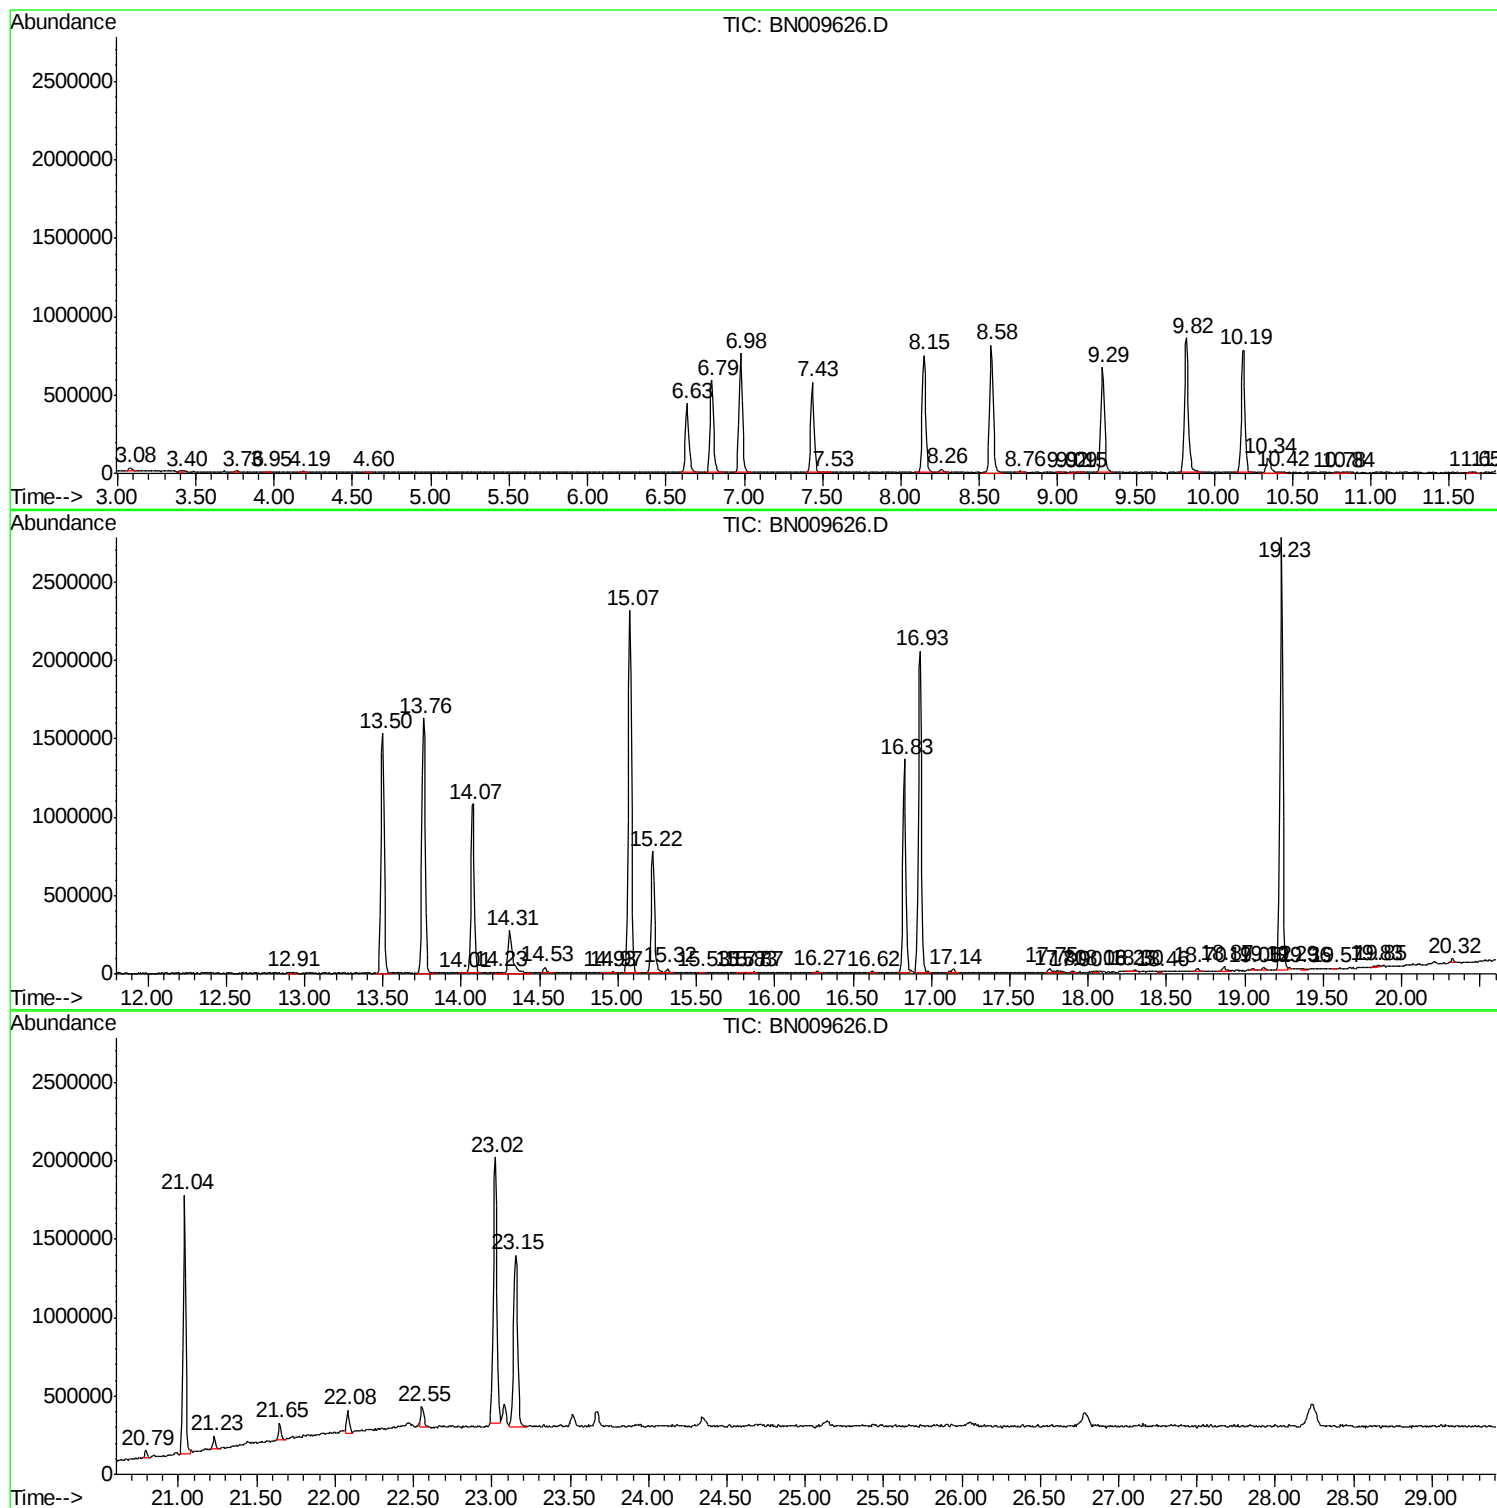

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020620\
Data File : BN009626.D
Acq On : 07 Feb 2020 01:11
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020620\
Data File : BN009626.D
Acq On : 07 Feb 2020 01:11
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc