
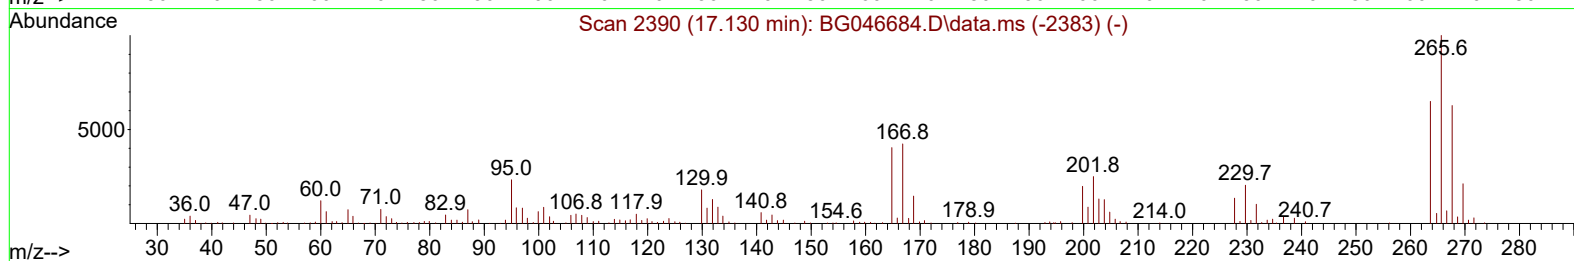
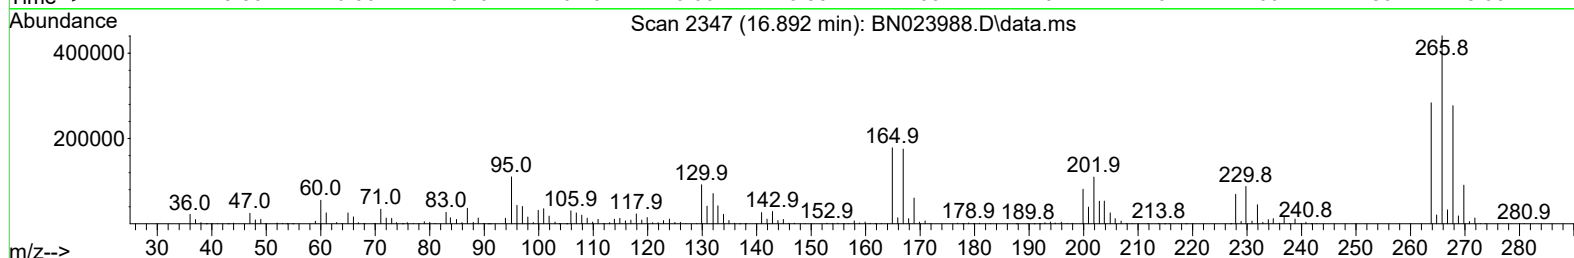


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020823\
Data File : BN023988.D
Acq On : 08 Feb 2023 13:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 04:12:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 09 04:12:09 2023
Response via : Initial Calibration

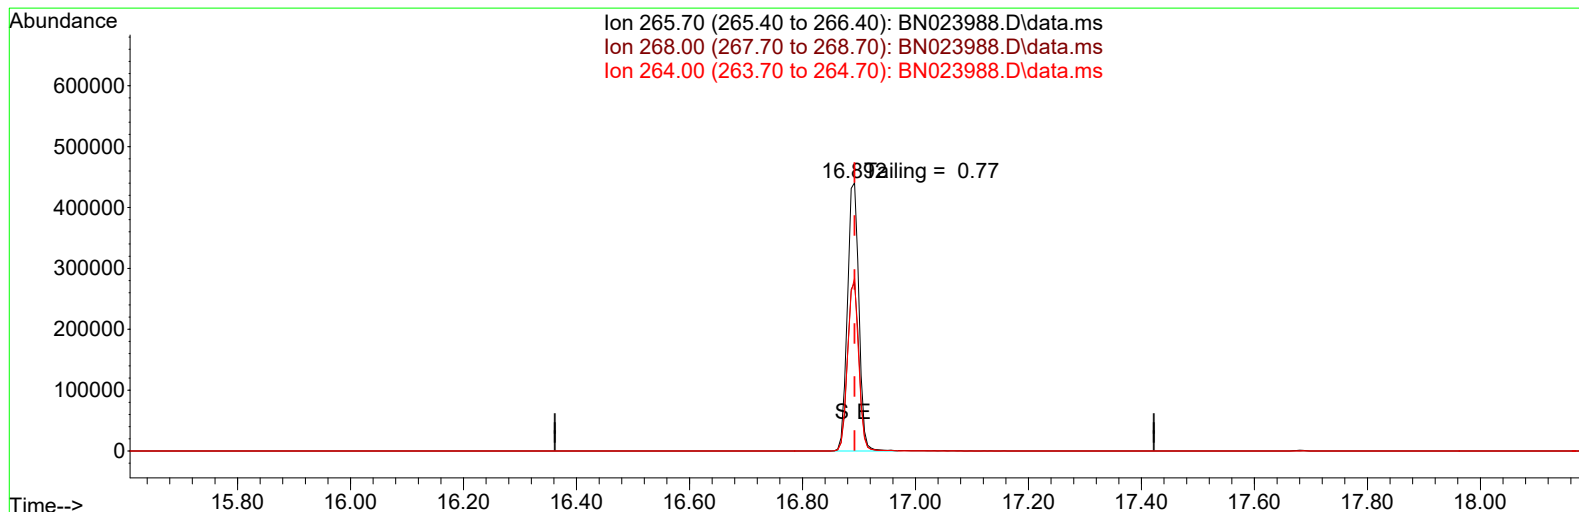

TIC: BN023988.D\data.ms

(70) Pentachlorophenol (C)




16.892min (0.000) 23672.13 ng

response 624197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.79
264.00	61.60	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020823\
Data File : BN023988.D
Acq On : 08 Feb 2023 13:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 04:12:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 09 04:12:09 2023
Response via : Initial Calibration

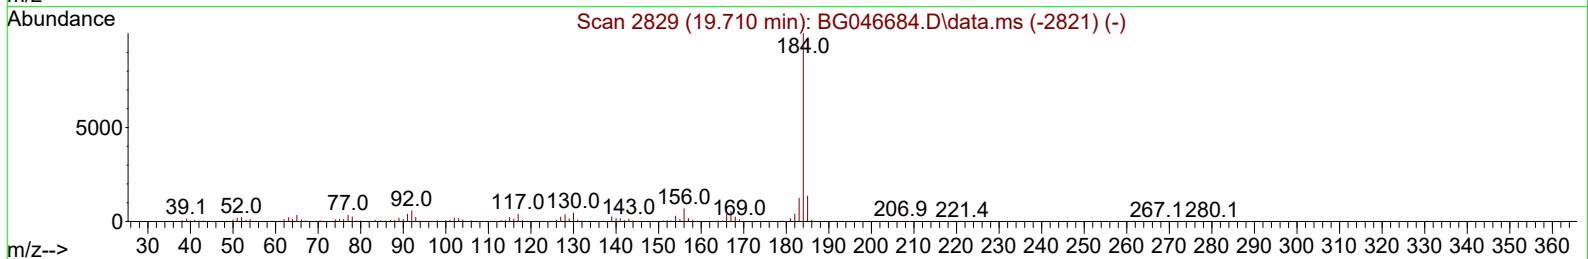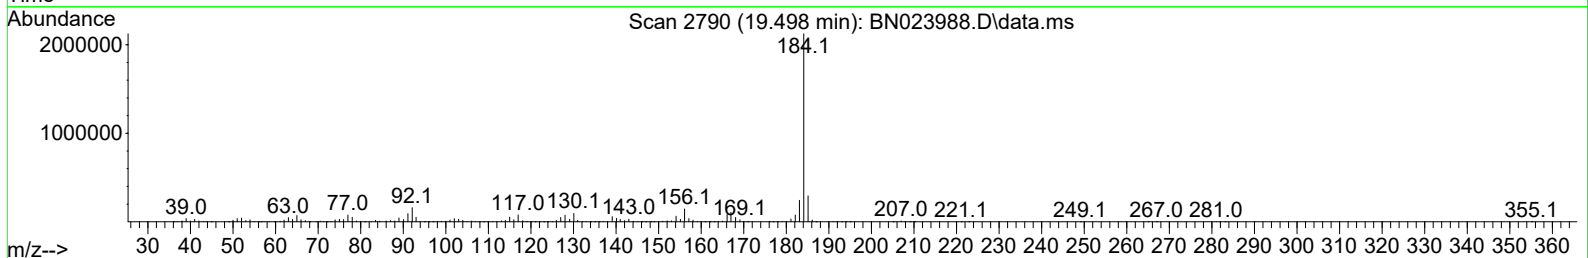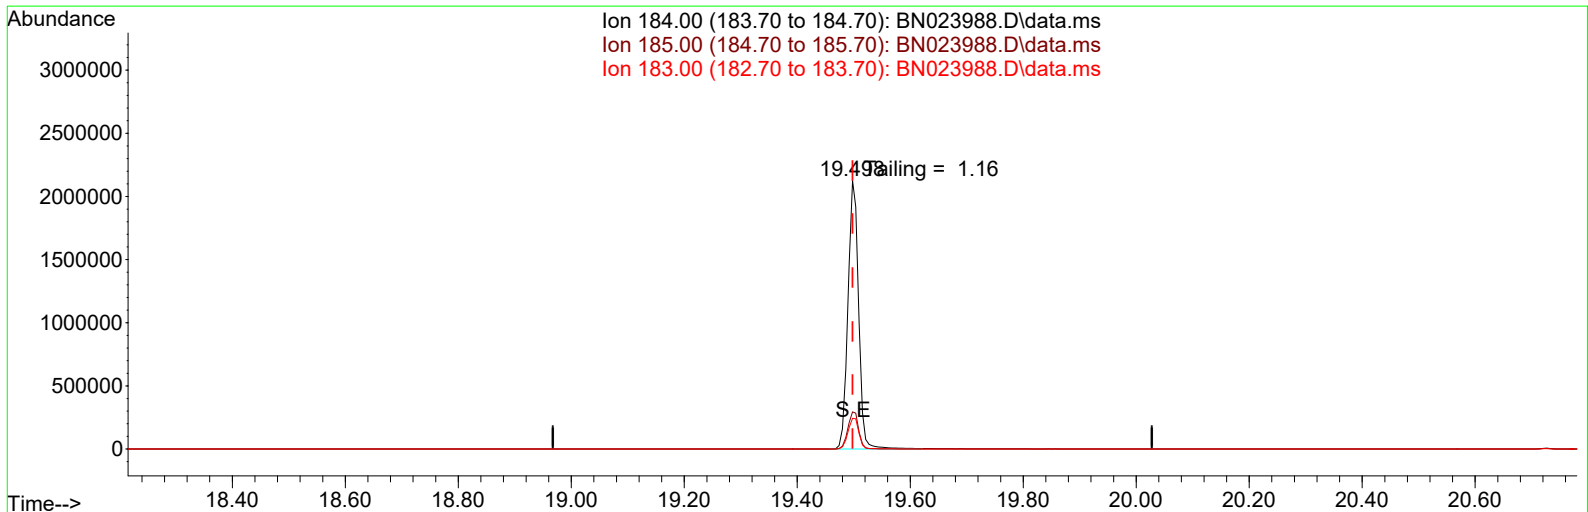

TIC: BN023988.D\data.ms

(77) Benzidine

19.498min (0.000) 0.00 ng

response 2794158

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.45
0.00	0.00	0.00