
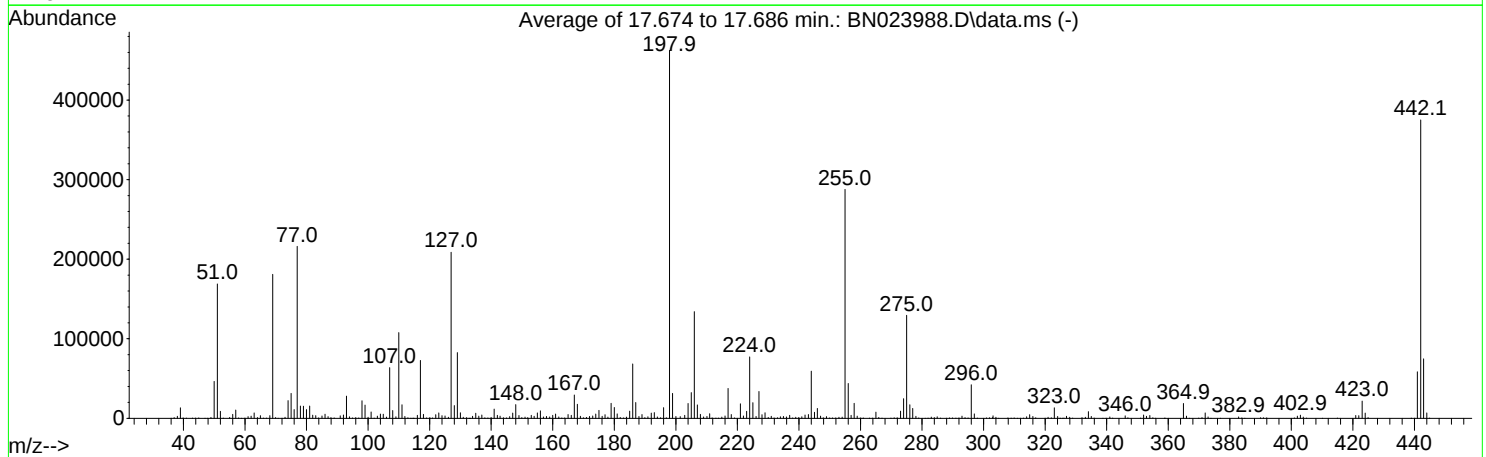


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN020823\  
 Data File : BN023988.D  
 Acq On : 08 Feb 2023 13:31  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN020723.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Feb 08 02:37:27 2023

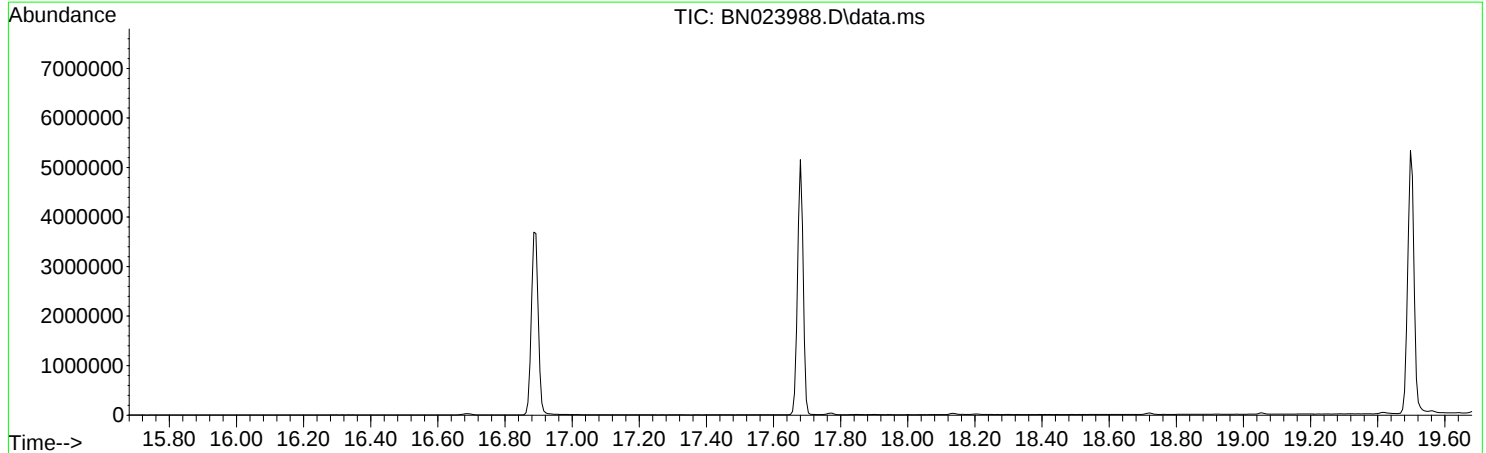




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.5         | 168840     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 3376       | PASS                |
| 69             | 198             | 0.00            | 100             | 39.1         | 181013     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 1006       | PASS                |
| 127            | 198             | 10              | 80              | 45.1         | 208725     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 812        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 462464     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 31384      | PASS                |
| 275            | 198             | 10              | 60              | 28.0         | 129384     | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 18575      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.6         | 58360      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 375104     | PASS                |
| 443            | 442             | 15              | 24              | 19.9         | 74664      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN020823\  
 Data File : BN023988.D  
 Acq On : 08 Feb 2023 13:31  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Feb 09 04:12:14 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 09 04:12:09 2023  
 Response via : Initial Calibration

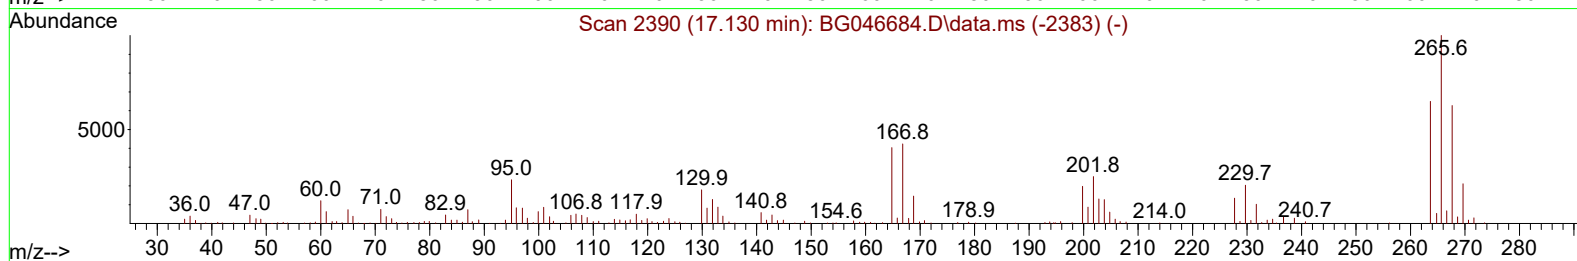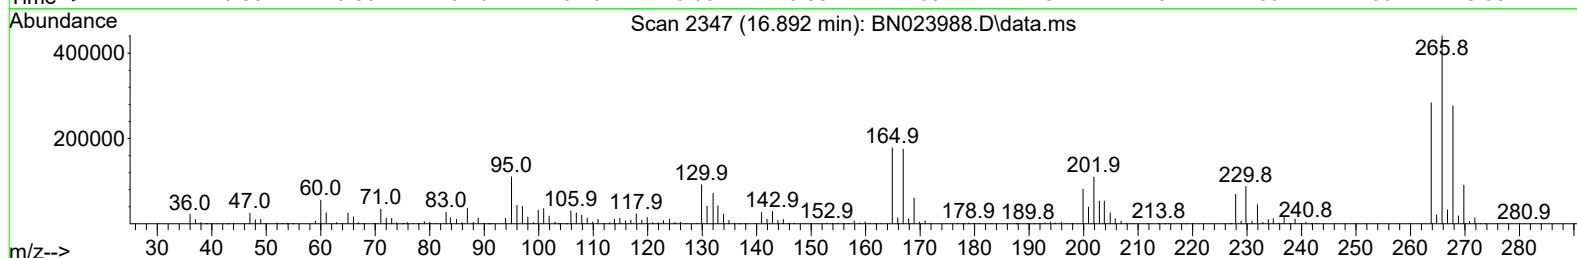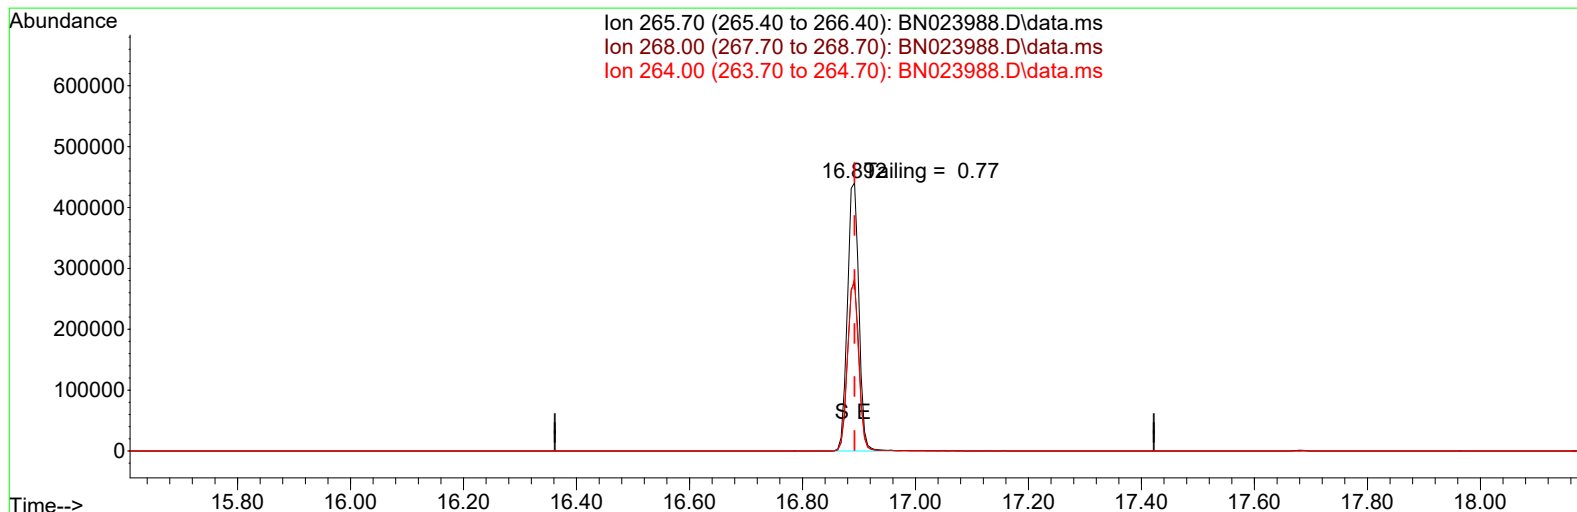

TIC: BN023988.D\data.ms

**(70) Pentachlorophenol (C)**

16.892min ( 0.000) 23672.13 ng




response 624197

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 62.79  |
| 264.00 | 61.60  | 64.33  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN020823\  
Data File : BN023988.D  
Acq On : 08 Feb 2023 13:31  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Feb 09 04:12:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 09 04:12:09 2023  
Response via : Initial Calibration

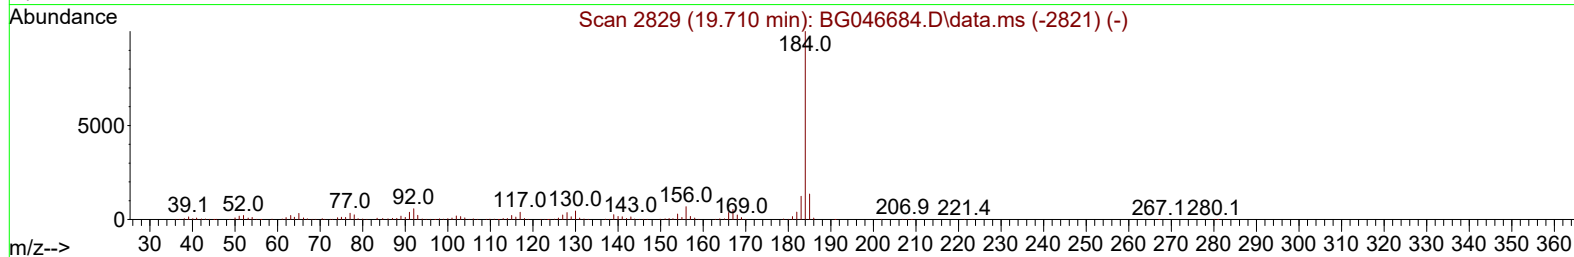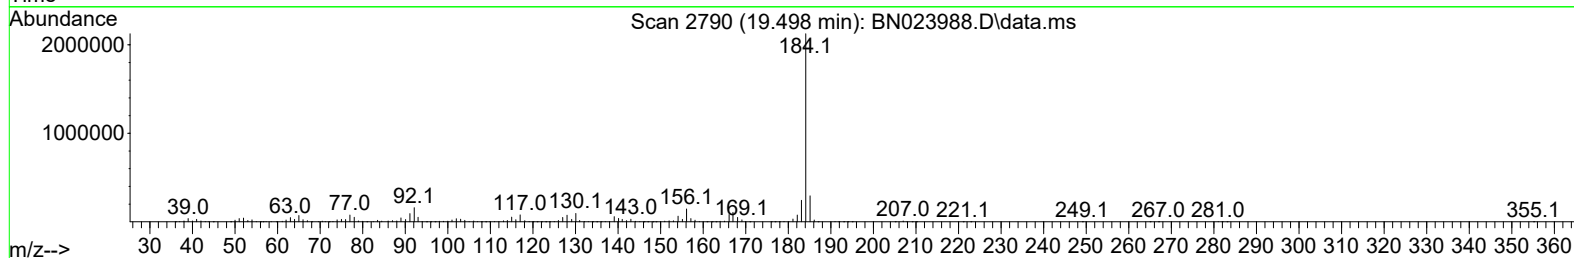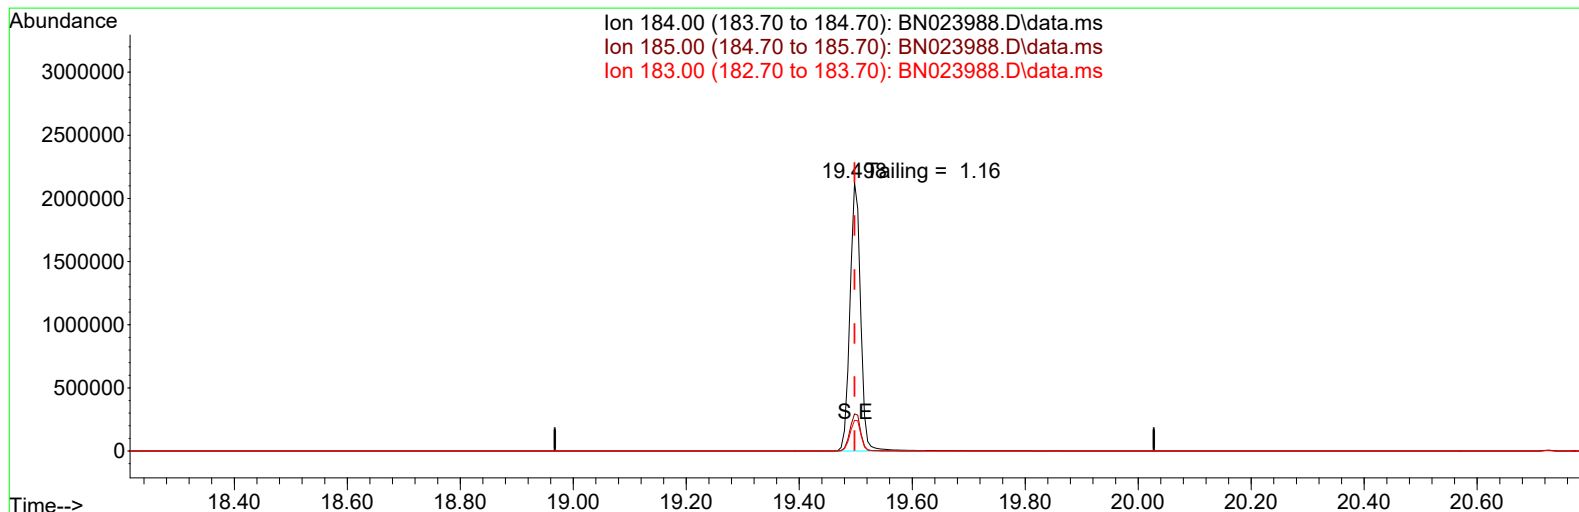

TIC: BN023988.D\data.ms

**(77) Benzidine**

**19.498min ( 0.000) 0.00 ng**

**response 2794158**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.82  |
| 183.00 | 13.20  | 11.45  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/8/2023      | BNA_N            | <u>BN023988.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1622225          | 20.727             |
| DDD           | 20486            | 20.333             |
| DDE           | 770              | 19.774             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 21256         | 1643481          | 1.29               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP