
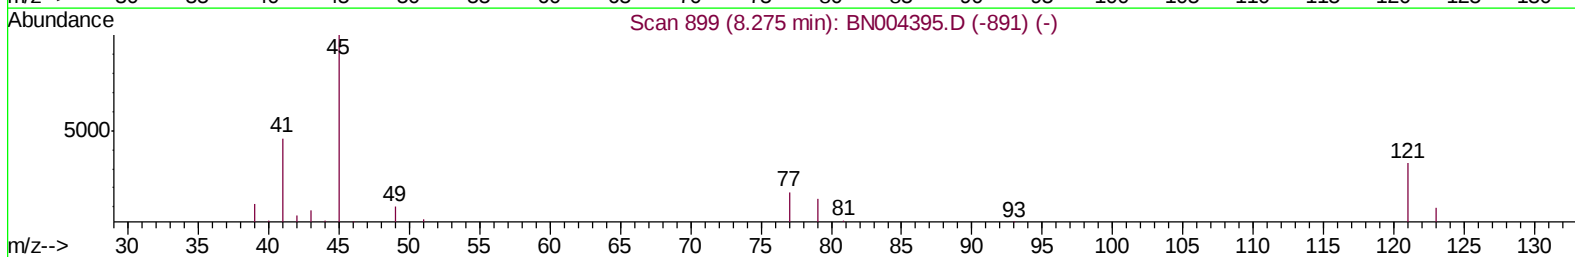
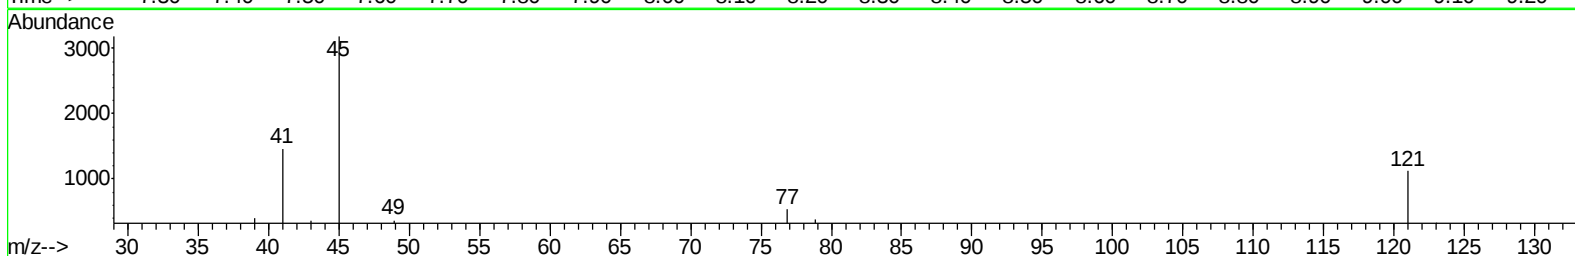


Data File : BN004400.D
Acq On : 13 Feb 2019 19:33
Operator : JU/SJ
Sample : MDL-S-05
Misc : 1PPM/4PPM
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Feb 14 06:48:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 14 06:43:40 2019
Response via : Initial Calibration

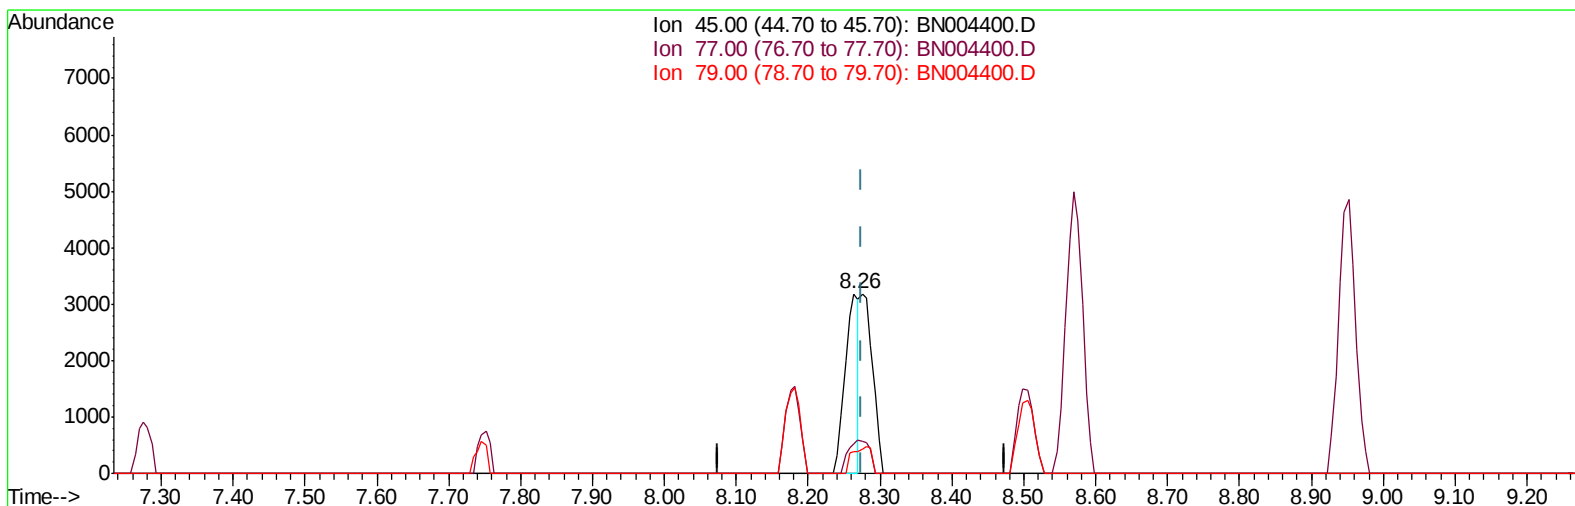

TIC: BN004400.D

(12) 2,2'-oxybis(1-Chloropropane)

8.263min (-0.012) 1.81ng/ul

response 4379

Ion	Exp%	Act%
45.00	100	100
77.00	17.60	16.65
79.00	13.50	12.00
0.00	0.00	0.00