

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021419\
 Data File : BN004420.D
 Acq On : 14 Feb 2019 15:05
 Operator : JU/SJ
 Sample : MDL-W-05
 Misc : 0.07 PPM
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-W-05

Quant Time: Feb 14 15:41:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 14:04:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	947	0.40	ng/ul	0.00
2) Naphthalene-d8	10.53	136	3736	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	2265	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	6405	0.40	ng/ul	0.00
16) Chrysene-d12	21.33	240	8232	0.40	ng/ul	0.00
20) Perylene-d12	23.60	264	8438	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	2072	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.16	212	6855	0.34	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.58	128	716	0.067	ng/ul#	81
5) 2-Methylnaphthalene	12.20	142	532	0.069	ng/ul	97
7) Acenaphthylene	14.11	152	624	0.060	ng/ul#	82
8) Acenaphthene	14.45	153	606	0.067	ng/ul	97
9) Fluorene	15.44	166	727	0.068	ng/ul#	97
11) Pentachlorophenol	16.78	266	39	0.029	ng/ul#	73
12) Phenanthrene	17.17	178	1377	0.066	ng/ul#	91
13) Anthracene	17.27	178	1105	0.063	ng/ul#	88
15) Fluoranthene	19.20	202	1745	0.068	ng/ul	93
17) Pyrene	19.56	202	1729	0.065	ng/ul#	93
18) Benzo(a)anthracene	21.31	228	1721	0.065	ng/ul	95
19) Chrysene	21.37	228	2148	0.070	ng/ul	96
21) Benzo(b)fluoranthene	22.91	252	2314	0.069	ng/ul	74
22) Benzo(k)fluoranthene	22.96	252	2164	0.065	ng/ul#	72
23) Benzo(a)pyrene	23.50	252	1906	0.063	ng/ul#	64
24) Indeno(1,2,3-cd)pyrene	25.89	276	2645	0.067	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.91	278	2077	0.065	ng/ul#	83
26) Benzo(g,h,i)perylene	26.59	276	2465	0.069	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021419\
Data File : BN004420.D
Acq On : 14 Feb 2019 15:05
Operator : JU/SJ
Sample : MDL-W-05
Misc : 0.07 PPM
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-W-05

Quant Time: Feb 14 15:41:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 14:04:55 2019
Response via : Initial Calibration

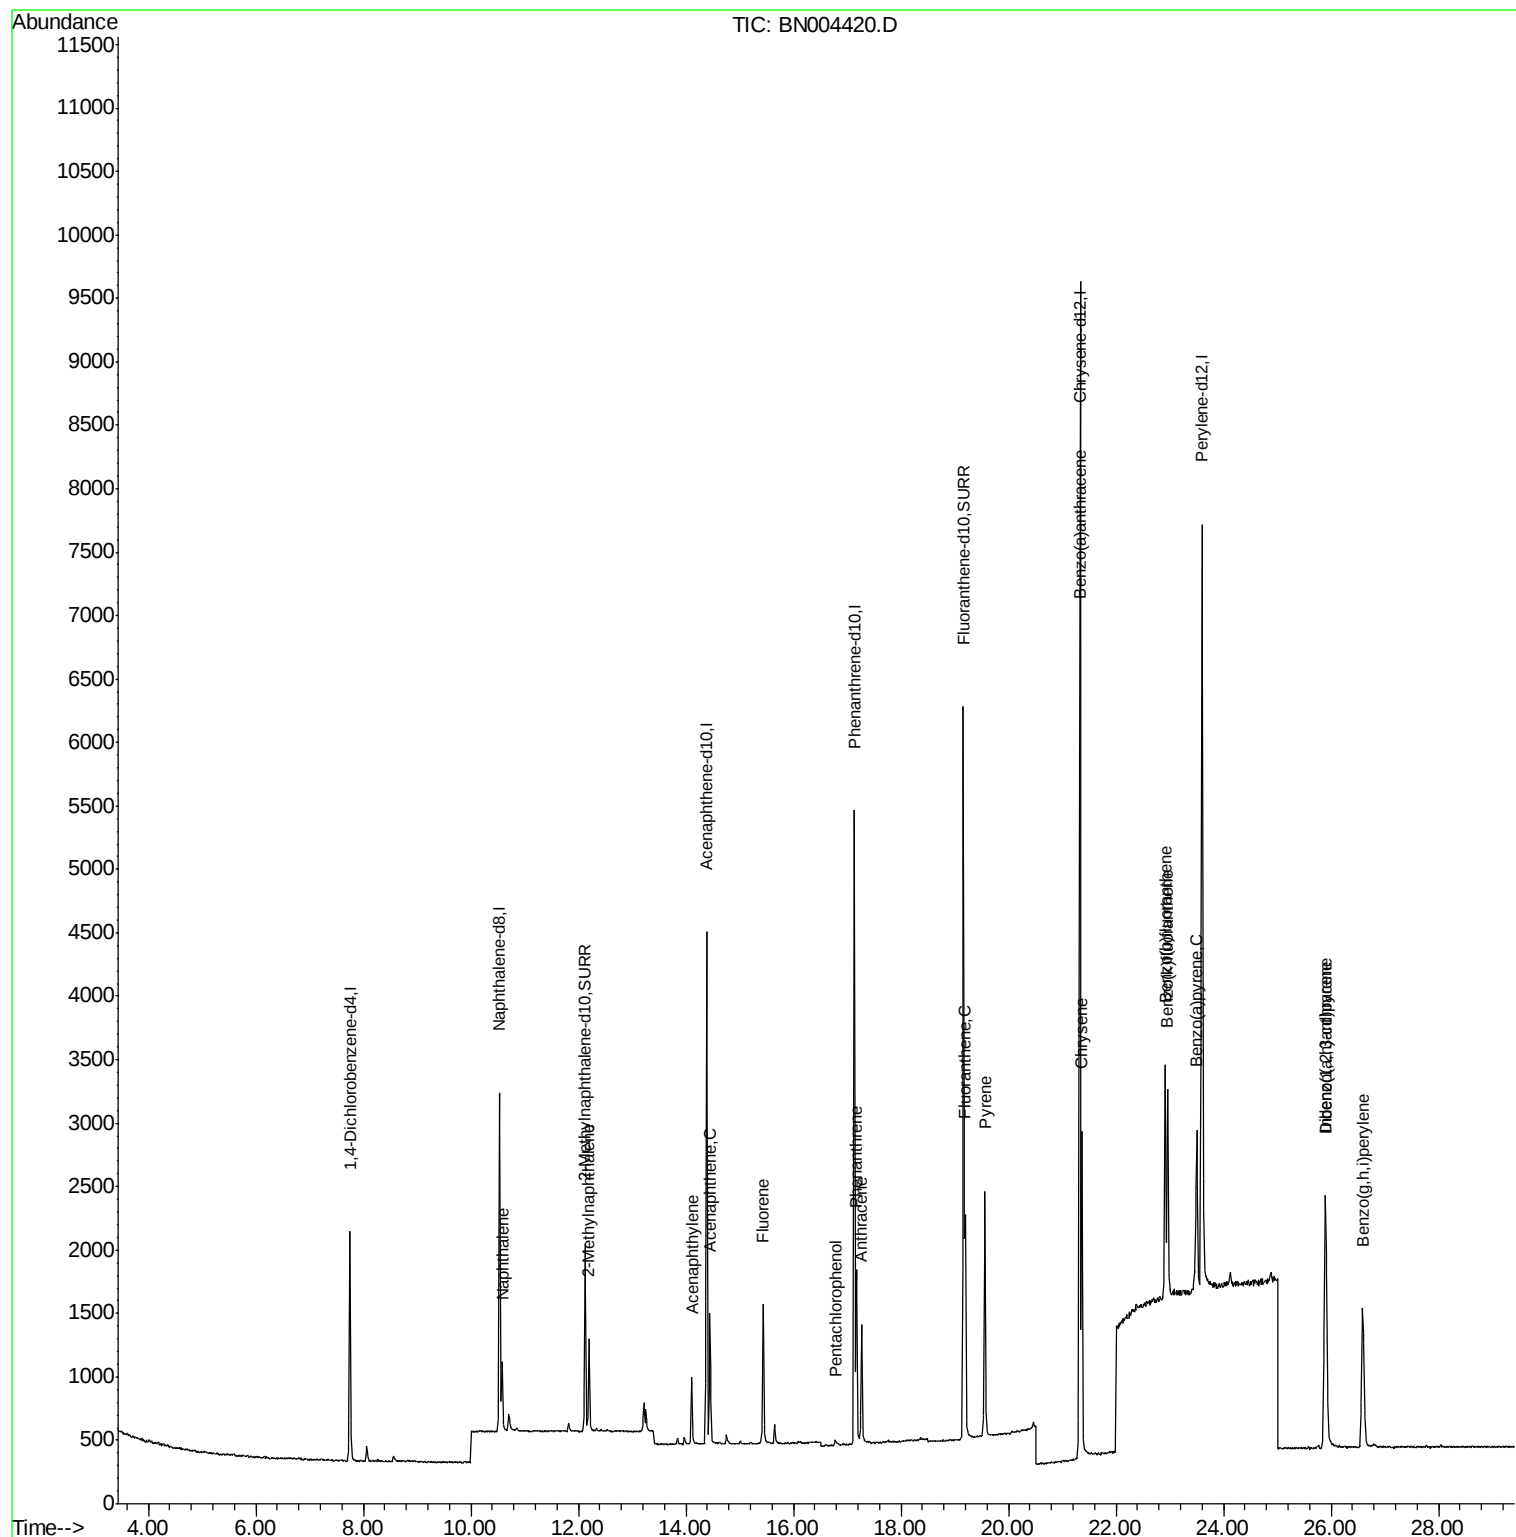



#3

Naphthalene

Concen: 0.067 ng/ul

RT: 10.58 min Scan# 2356

Delta R.T. -0.01 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:128 Resp: 716

Ion Ratio Lower Upper

128 100

129 19.8 9.8 14.6#




127 21.6 11.4 17.0#

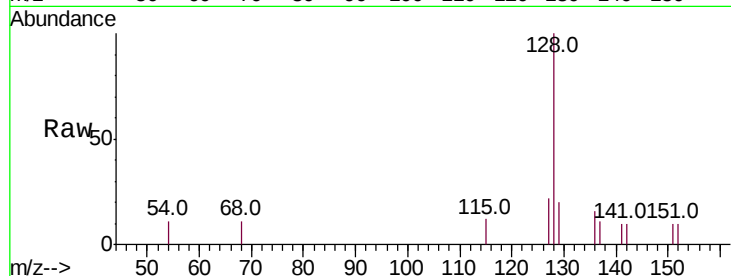

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

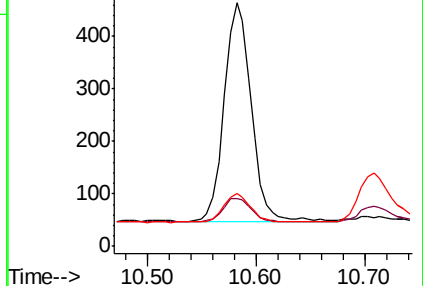

#5

2-Methylnaphthalene

Concen: 0.069 ng/ul

RT: 12.20 min Scan# 2650

Delta R.T. -0.01 min

Lab File: BN004420.D


Acq: 14 Feb 2019 15:05

Tgt Ion:142 Resp: 532

Ion Ratio Lower Upper



142 100


141 87.0 71.8 107.6



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

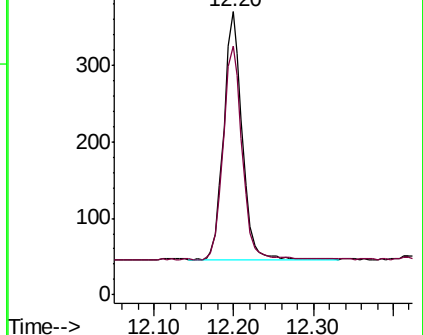



#7

Acenaphthylene

Concen: 0.060 ng/ul

RT: 14.11 min Scan# 3021

Delta R.T. -0.01 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:152 Resp: 624

Ion Ratio Lower Upper

152 100

151 28.2 16.6 24.8#




153 22.5 11.1 16.7#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

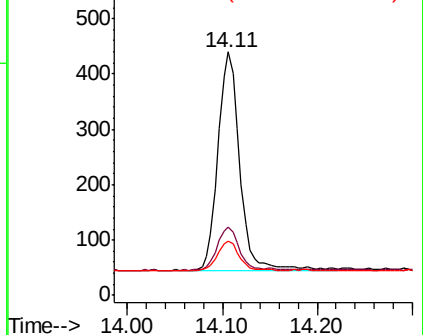

#8

Acenaphthene

Concen: 0.067 ng/ul

RT: 14.45 min Scan# 3095

Delta R.T. -0.01 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:153 Resp: 606

Ion Ratio Lower Upper

153 100

152 53.3 38.4 57.6



154 89.9 71.4 107.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E




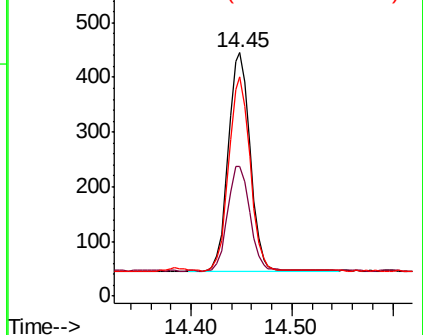




#9
Fluorene
 Concen: 0.068 ng/ul
 RT: 15.44 min Scan# 3309
 Delta R.T. -0.00 min
 Lab File: BN004420.D
 Acq: 14 Feb 2019 15:05




Instrument :
 BNA_N
 ClientSampleId :
 MDL-W-05


Tot Ion:166 Resp: 727
 Ion Ratio Lower Upper
 166 100
 165 100.0 78.9 118.3
 167 20.4 11.6 17.4#

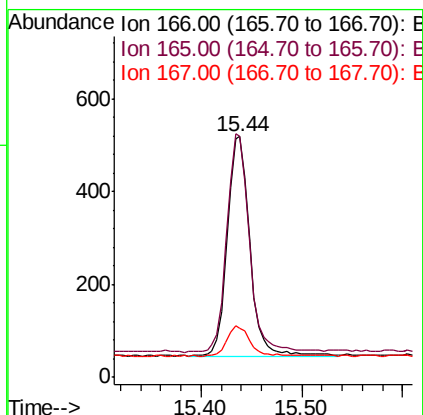

#11
Pentachlorophenol
 Concen: 0.029 ng/ul
 RT: 16.78 min Scan# 3605
 Delta R.T. 0.00 min
 Lab File: BN004420.D
 Acq: 14 Feb 2019 15:05

Tgt Ion:266 Resp: 39
 Ion Ratio Lower Upper
 266 100
 264 74.4 52.3 78.5
 268 94.9 49.0 73.6#

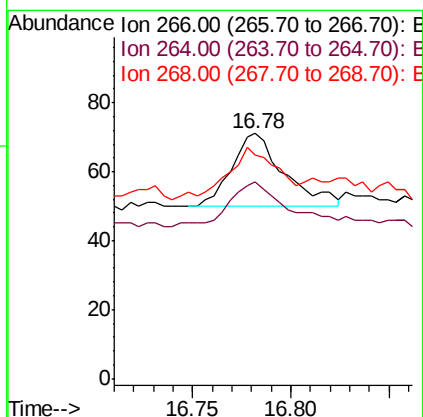

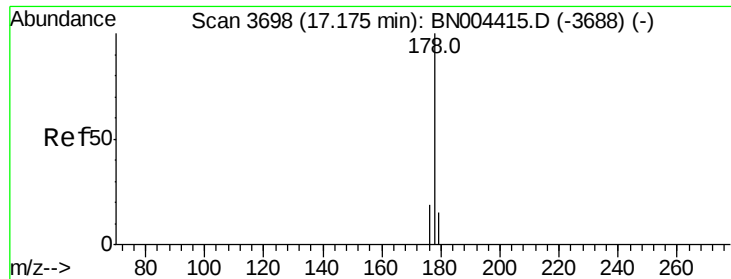

#12

Phenanthrene

Concen: 0.066 ng/ul

RT: 17.17 min Scan# 3698

Delta R.T. -0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:178 Resp: 1377

Ion Ratio Lower Upper

178 100

179 20.3 12.6 19.0#




176 22.9 15.8 23.6



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

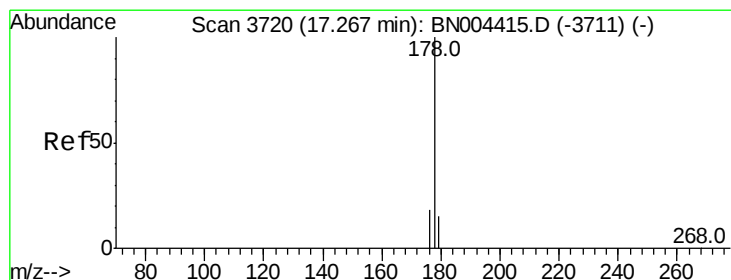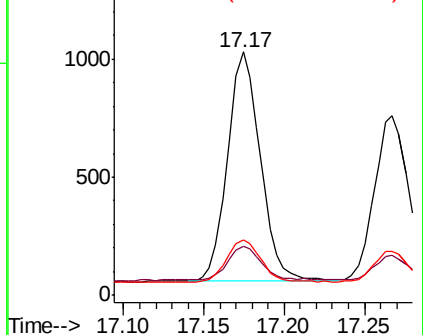

#13

Anthracene

Concen: 0.063 ng/ul

RT: 17.27 min Scan# 3720

Delta R.T. -0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:178 Resp: 1105

Ion Ratio Lower Upper

178 100

179 22.0 13.0 19.4#



176 24.3 15.5 23.3#




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

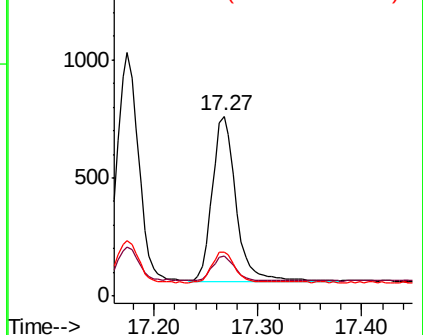

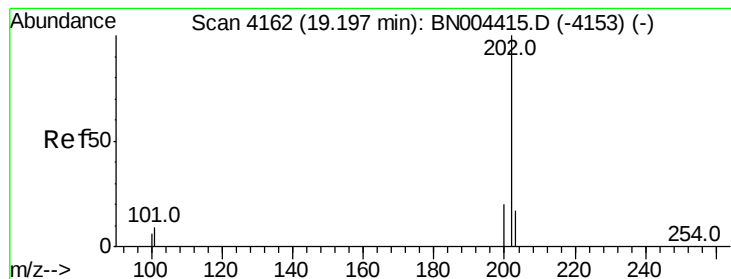

#15

Fluoranthene

Concen: 0.068 ng/ul

RT: 19.20 min Scan# 4162

Delta R.T. -0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:202 Resp: 1745

Ion Ratio Lower Upper

202 100

101 12.7 0.0 30.4




100 10.2 0.0 27.6

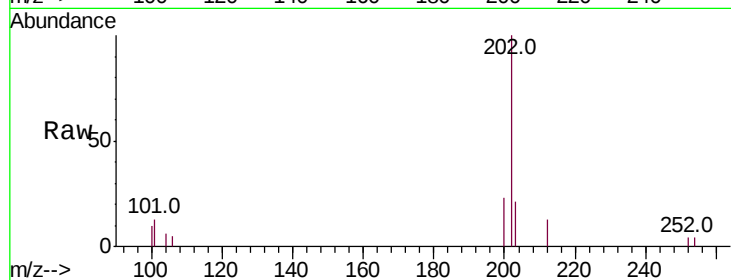

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

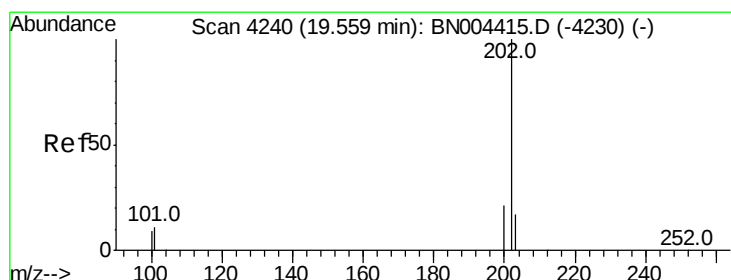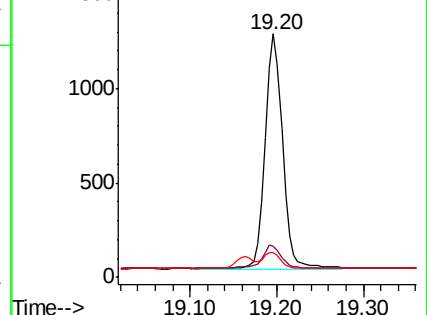

#17

Pyrene

Concen: 0.065 ng/ul

RT: 19.56 min Scan# 4241

Delta R.T. -0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:202 Resp: 1729

Ion Ratio Lower Upper

202 100

101 13.9 9.0 13.6#



100 11.6 7.4 11.0#

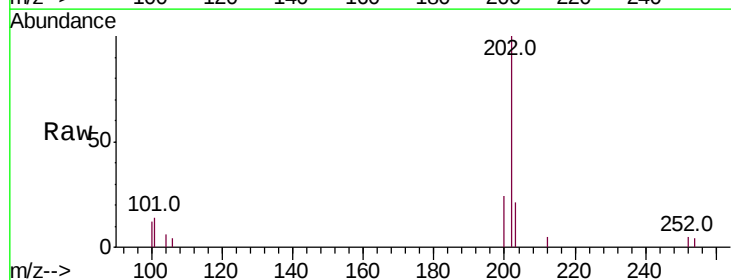


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

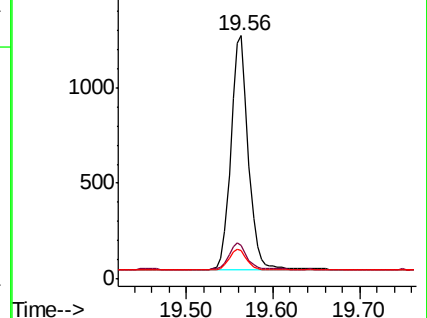

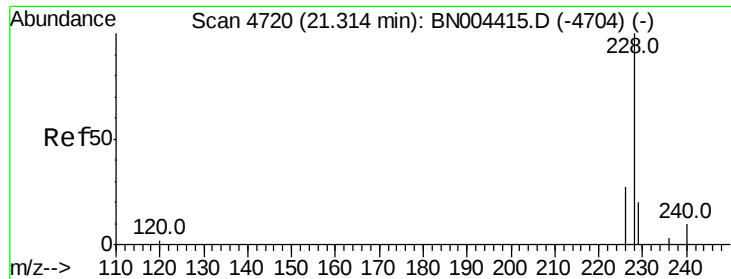

#18

Benzo(a)anthracene

Concen: 0.065 ng/ul

RT: 21.31 min Scan# 4720

Delta R.T. -0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:228 Resp: 1721

Ion Ratio Lower Upper




228 100

229 22.2 15.7 23.5

226 29.8 22.1 33.1



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

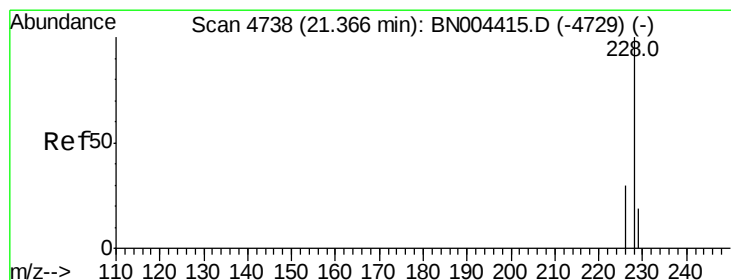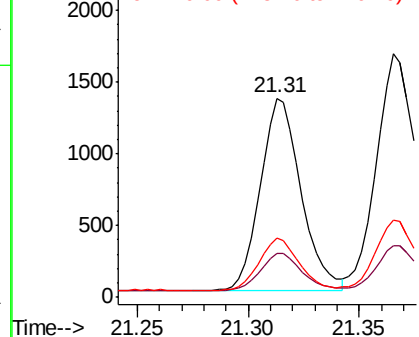

#19

Chrysene

Concen: 0.070 ng/ul

RT: 21.37 min Scan# 4738

Delta R.T. -0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:228 Resp: 2148

Ion Ratio Lower Upper



228 100


226 31.8 23.8 35.8

229 21.2 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

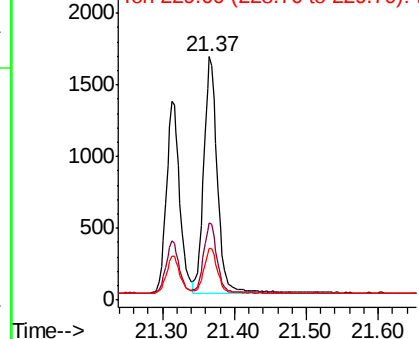

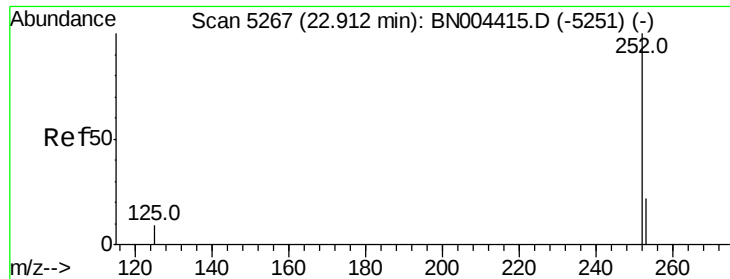

#21

Benzo(b)fluoranthene

Concen: 0.069 ng/ul

RT: 22.91 min Scan# 5268

Delta R.T. 0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:252 Resp: 2314

Ion Ratio Lower Upper

252 100

253 38.1 0.0 48.0




125 19.6 0.0 22.8

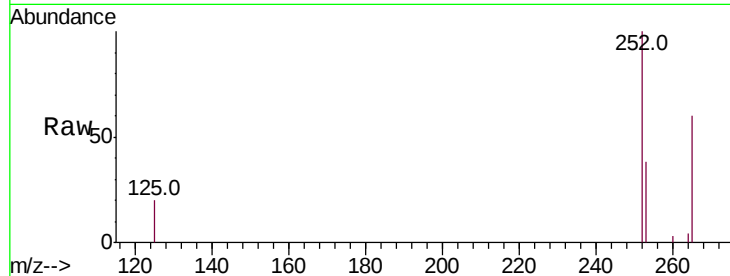

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

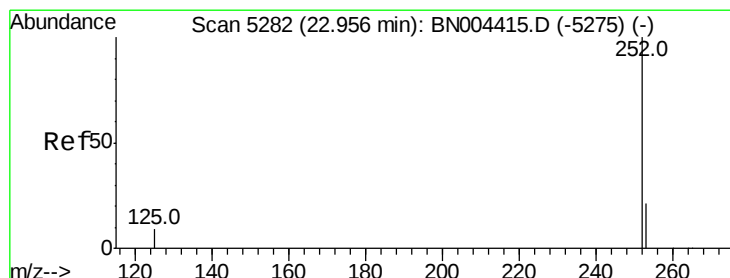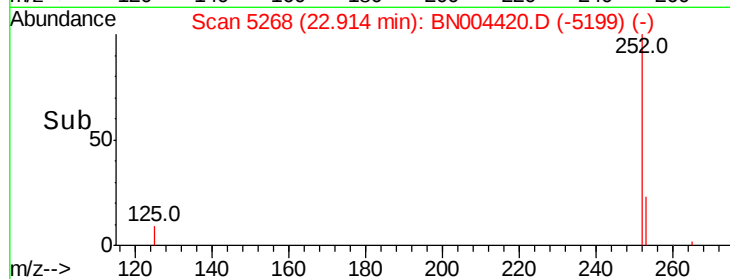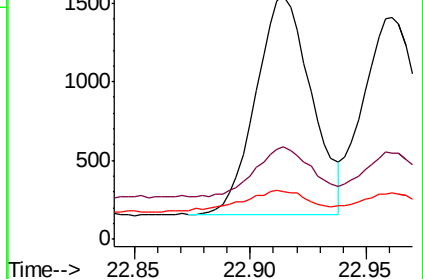

#22

Benzo(k)fluoranthene

Concen: 0.065 ng/ul

RT: 22.96 min Scan# 5284

Delta R.T. 0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:252 Resp: 2164

Ion Ratio Lower Upper

252 100

253 38.7 19.5 29.3#



125 20.9 9.1 13.7#

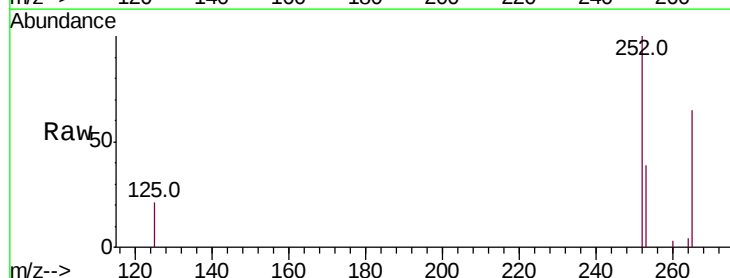


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

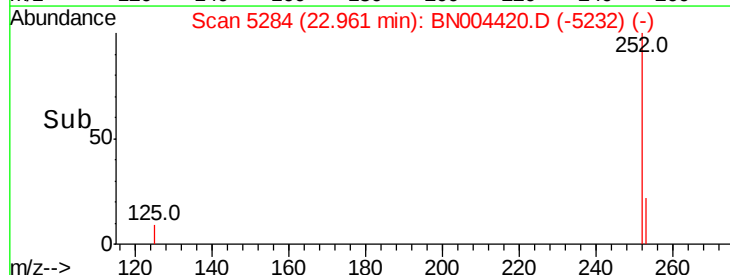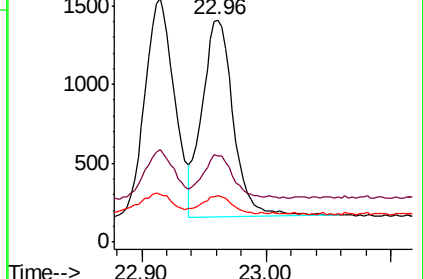

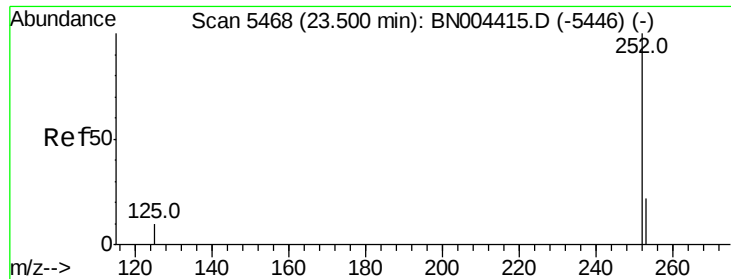

#23

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 23.50 min Scan# 5468

Delta R.T. 0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:252 Resp: 1906

Ion Ratio Lower Upper

252 100

253 44.6 20.4 30.6#




125 25.9 10.6 15.8#

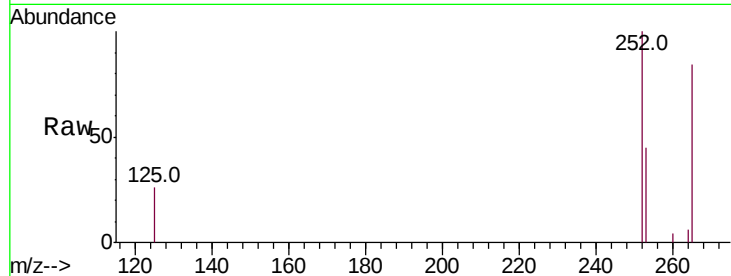

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

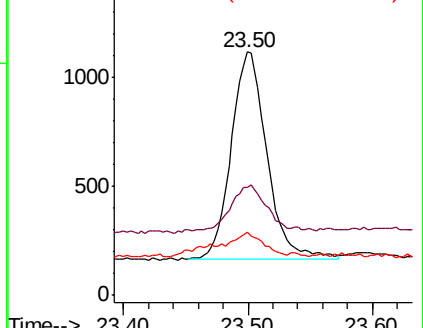

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.067 ng/ul

RT: 25.89 min Scan# 6247

Delta R.T. 0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:276 Resp: 2645

Ion Ratio Lower Upper

276 100

138 23.2 19.1 28.7



227 0.2 0.2 0.4#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

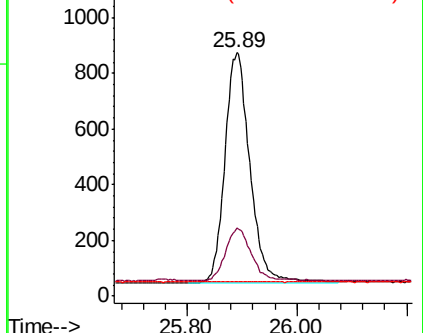



#25

Dibenzo(a,h)anthracene

Concen: 0.065 ng/u1

RT: 25.91 min Scan# 6252

Delta R.T. 0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05

Instrument :

BNA_N

ClientSampleId :

MDL-W-05


Tot Ion:278 Resp: 2077

Ion Ratio Lower Upper

278 100

139 21.5 13.8 20.6#




279 36.9 20.4 30.6#

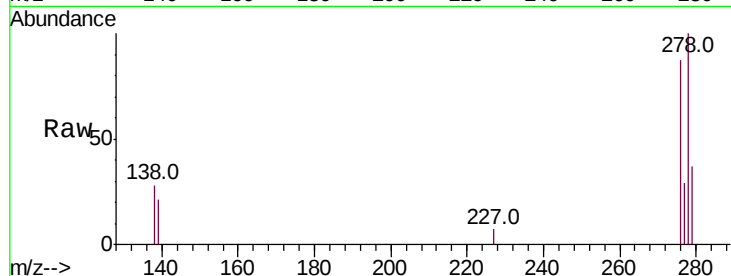

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

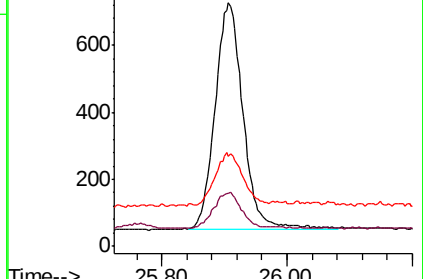

#26

Benzo(g,h,i)perylene

Concen: 0.069 ng/u1

RT: 26.59 min Scan# 6457

Delta R.T. 0.00 min

Lab File: BN004420.D

Acq: 14 Feb 2019 15:05


Tgt Ion:276 Resp: 2465

Ion Ratio Lower Upper

276 100

138 25.4 16.8 25.2#

277 29.8 19.4 29.0#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

