


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021819\
Data File : BN004434.D
Acq On : 18 Feb 2019 10:05
Operator : JU/SJ
Sample : DFTPP04
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP04

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION
Last Update : Thu Feb 14 07:13:45 2019

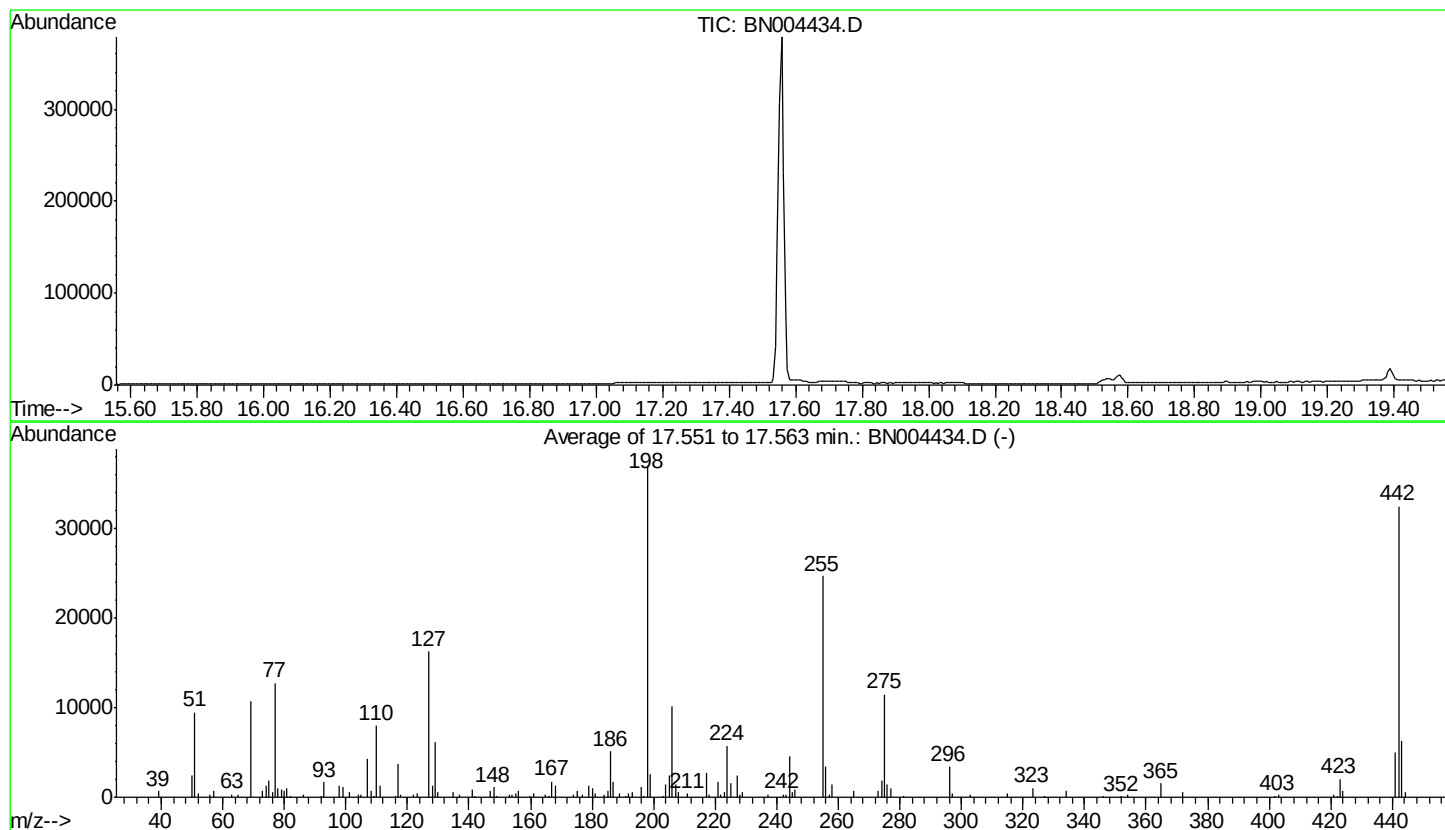

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	9462	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.9	10694	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	16233	PASS
197	198	0.00	2	0.3	105	PASS
198	198	100	100	100.0	36986	PASS
199	198	5	9	6.9	2554	PASS
275	198	10	60	31.0	11472	PASS
365	198	1	100	4.2	1563	PASS
441	198	0.01	100	13.7	5067	PASS
442	198	50	100	87.8	32456	PASS
443	442	15	24	19.3	6256	PASS

Scan 2471 (17.522 min): BN004434.D
DFTPP04

m/z	Abundance
44.00	633.0
185.00	466.0
186.00	560.0
207.00	817.0

Instrument :
BNA_N
ClientSampleId :
DFTPP04

m/z	Abundance
39.00	819.0
44.00	659.0
50.00	3003.0
51.00	11160.0
52.00	622.0
55.90	357.0
57.00	802.0
63.00	477.0
65.00	326.0
69.00	12423.0
73.00	396.0
74.00	1442.0
75.00	2191.0
76.00	678.0
77.00	14533.0
78.00	1166.0
79.00	1039.0
80.00	761.0
80.90	1115.0
86.00	423.0
91.90	324.0
93.00	1868.0
98.00	1499.0
99.00	1418.0
101.00	561.0
104.00	416.0
105.00	413.0
107.00	4776.0
108.00	834.0
110.00	8840.0
111.00	1431.0
117.00	4039.0
118.00	321.0
121.90	353.0
123.00	502.0
127.00	17872.0
128.00	1341.0
129.00	6672.0
129.90	566.0
135.00	624.0
136.90	415.0
141.00	1025.0
142.00	310.0
147.00	612.0
148.00	1179.0
149.00	330.0
153.00	363.0
153.90	332.0
155.00	497.0
156.00	744.0
160.00	301.0
160.90	467.0
164.90	388.0
166.00	308.0
167.00	1700.0
168.00	1543.0
174.00	448.0
175.00	707.0
176.90	389.0
178.90	1324.0
180.00	1063.0
181.00	424.0
184.10	312.0
185.00	1206.0
186.00	5888.0
187.00	1737.0
189.00	400.0
192.00	417.0
193.00	583.0
196.00	1033.0
198.00	37600.0
199.00	2751.0
204.00	1364.0
205.00	2428.0
206.00	9972.0
207.00	2328.0
208.00	553.0
211.00	423.0
217.00	2734.0
218.00	350.0
221.00	1746.0
221.80	412.0
222.90	610.0
224.00	5827.0
225.00	1635.0
227.00	2467.0
228.00	325.0
229.00	510.0
237.00	378.0
241.90	334.0
243.00	321.0

Instrument :
BNA_N
ClientSampleId :
DFTPP04

244.00	4434.0
245.00	623.0
246.00	851.0
255.00	23144.0
256.00	3389.0
257.00	374.0
258.00	1343.0
264.90	616.0
273.00	699.0
274.00	1868.0
275.00	10691.0
276.00	1415.0
277.00	862.0
296.00	2986.0
297.00	332.0
303.00	327.0
314.90	350.0
323.10	850.0
334.00	642.0
365.00	1418.0
372.00	553.0
423.00	1504.0
424.00	681.0
441.00	4104.0
442.00	25704.0
443.00	5003.0
444.10	515.0

Instrument :
BNA_N
ClientSampleId :
DFTPP04

m/z	Abundance
39.00	797.0
43.90	669.0
50.00	2847.0
51.00	11211.0
52.00	624.0
55.90	358.0
57.00	876.0
63.00	505.0
65.00	353.0
69.00	13025.0
73.00	698.0
74.00	1501.0
75.00	2255.0
76.00	711.0
77.00	15503.0
78.00	1112.0
79.00	1068.0
79.90	822.0
81.00	1113.0
81.90	340.0
86.00	342.0
92.00	305.0
93.00	1944.0
98.00	1587.0
99.00	1350.0
100.90	626.0
104.00	457.0
105.00	370.0
107.00	5336.0
108.00	842.0
109.00	305.0
110.00	9800.0
111.00	1548.0
116.00	330.0
117.00	4701.0
117.90	365.0
121.90	337.0
123.00	657.0
127.00	19984.0
128.00	1501.0
129.00	7427.0
129.90	728.0
135.00	661.0
136.90	406.0
141.00	1068.0
142.00	346.0
147.00	786.0
148.00	1331.0
149.00	329.0
153.00	333.0
154.00	379.0
155.00	543.0
156.00	959.0
159.90	321.0
161.00	513.0
165.00	465.0
167.00	2197.0
168.00	1579.0
174.00	457.0
175.00	869.0
176.90	466.0
179.00	1568.0
180.00	1310.0
181.00	538.0
184.00	353.0
185.00	1380.0
186.00	6778.0
187.00	2181.0
188.90	422.0
191.10	327.0
192.00	541.0
193.00	649.0
196.00	1433.0
196.90	315.0
198.00	45984.0
199.00	3077.0
203.00	311.0
204.00	1784.0
205.00	2880.0
206.00	12529.0
207.00	2559.0
208.00	670.0
211.10	488.0
217.00	3389.0
217.90	483.0
221.00	2235.0
221.90	566.0
223.00	746.0
224.00	7186.0
225.00	1952.0
227.00	3051.0

Instrument :
BNA_N
ClientSampleId :
DFTPP04

228.00	392.0
228.90	658.0
237.00	433.0
242.00	408.0
243.10	384.0
244.00	5576.0
245.00	739.0
246.00	1199.0
255.00	31224.0
256.00	4270.0
257.00	483.0
258.00	1808.0
264.90	853.0
272.90	937.0
274.00	2277.0
275.00	14304.0
276.00	1727.0
277.00	1340.0
296.00	4255.0
297.10	616.0
303.00	410.0
314.90	430.0
323.00	1330.0
326.90	309.0
334.00	881.0
345.90	332.0
352.00	403.0
354.00	438.0
365.00	1860.0
372.00	716.0
402.00	320.0
403.00	491.0
421.00	446.0
422.00	409.0
423.00	2431.0
424.10	927.0
441.10	6047.0
442.00	39304.0
443.00	7713.0
444.00	660.0

Instrument :

BNA_N

ClientSampleId :

DFTPP04

m/z	Abundance
39.00	439.0
44.00	632.0
50.00	1578.0
51.00	6017.0
57.00	430.0
69.00	6635.0
73.10	902.0
74.00	855.0
75.00	1120.0
76.00	338.0
77.00	8124.0
78.00	638.0
78.90	590.0
80.00	398.0
80.90	603.0
93.00	1144.0
98.00	811.0
99.00	716.0
101.00	358.0
107.00	2913.0
108.00	433.0
110.00	5177.0
110.90	807.0
117.00	2413.0
122.90	318.0
127.00	10844.0
128.00	822.0
129.00	4384.0
129.90	355.0
134.90	384.0
141.00	665.0
147.00	803.0
148.00	765.0
155.00	325.0
155.90	496.0
161.00	331.0
167.00	1304.0
168.00	931.0
175.00	539.0
178.90	962.0
180.00	741.0
180.90	356.0
184.00	372.0
185.00	978.0
186.00	4335.0
187.00	1229.0
189.00	325.0
191.90	333.0
193.00	377.0
196.00	807.0
198.00	27376.0
199.00	1836.0
204.00	1005.0
205.10	1848.0
206.00	7818.0
207.00	1847.0
208.00	445.0
210.90	304.0
217.00	2003.0
221.00	1382.0
223.00	557.0
224.00	4304.0
225.00	1079.0
227.00	1739.0
229.00	406.0
242.00	315.0
243.00	332.0
244.00	3600.0
245.00	456.0
246.00	689.0
255.00	19584.0
256.00	2695.0
258.00	1241.0
265.00	554.0
273.00	634.0
274.00	1618.0
275.00	9423.0
276.00	1128.0
276.90	848.0
281.00	433.0
296.00	2962.0
297.00	466.0
303.00	321.0
315.00	313.0
323.00	910.0
334.00	584.0
354.00	348.0
365.00	1413.0
372.00	540.0
402.90	365.0
421.00	301.0

Instrument :
BNA_N
ClientSampleId :
DFTPP04

423.00	2070.0
424.00	702.0
441.00	5052.0
442.00	32360.0
443.00	6052.0
444.00	533.0

Instrument :
BNA_N
ClientSampleId :
DFTPP04