


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021919\
Data File : BN004458.D
Acq On : 19 Feb 2019 14:04
Operator : JU/SJ
Sample : K1455-01 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BE801

Manual Integrations
APPROVED

Sohil
2/20/2019 2:08:12 PM

Quant Time: Feb 19 15:05:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 19 14:16:20 2019
Response via : Initial Calibration

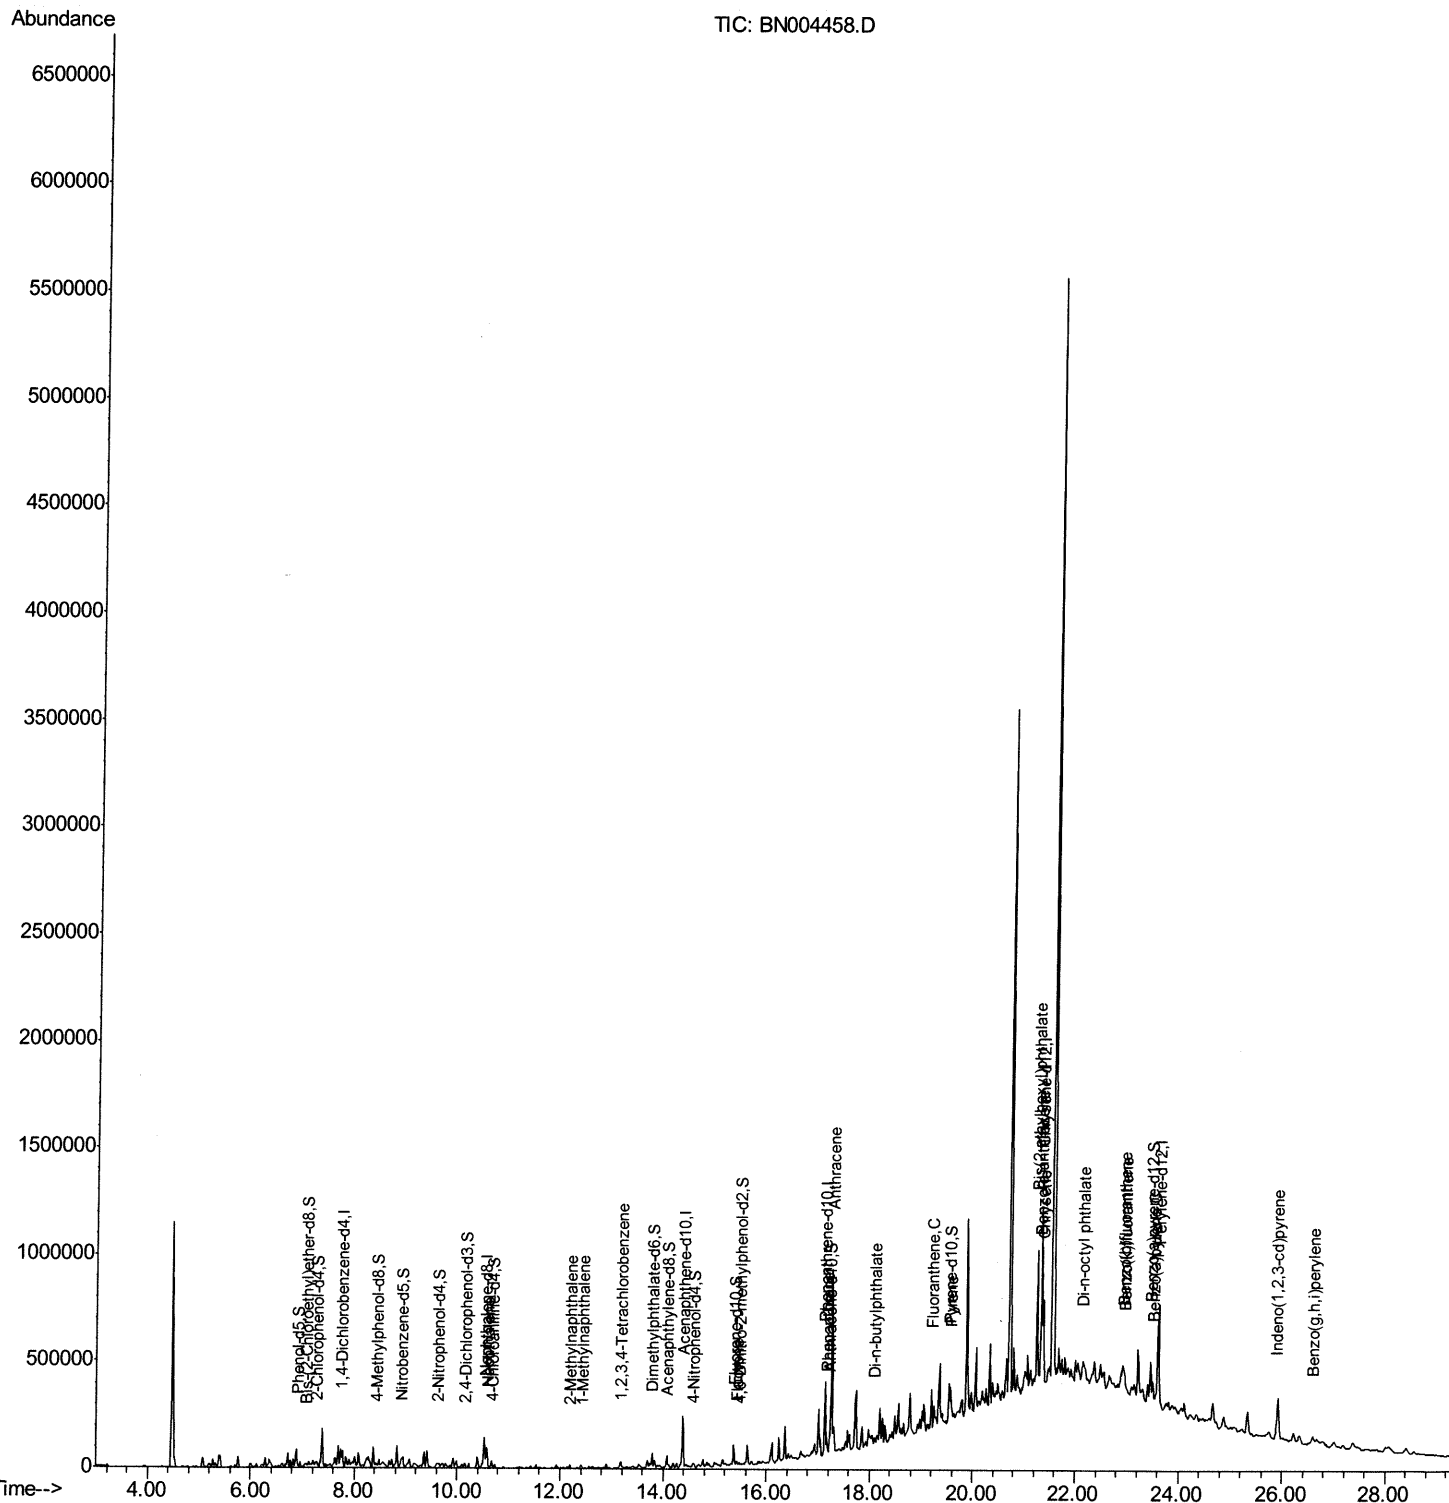




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021919\
Data File : BN004458.D
Acq On : 19 Feb 2019 14:04
Operator : JU/SJ
Sample : K1455-01 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BE801

Manual Integrations
APPROVED

Sohil
2/20/2019 2:08:12 PM

Quant Time: Feb 19 14:56:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 19 14:16:20 2019
Response via : Initial Calibration

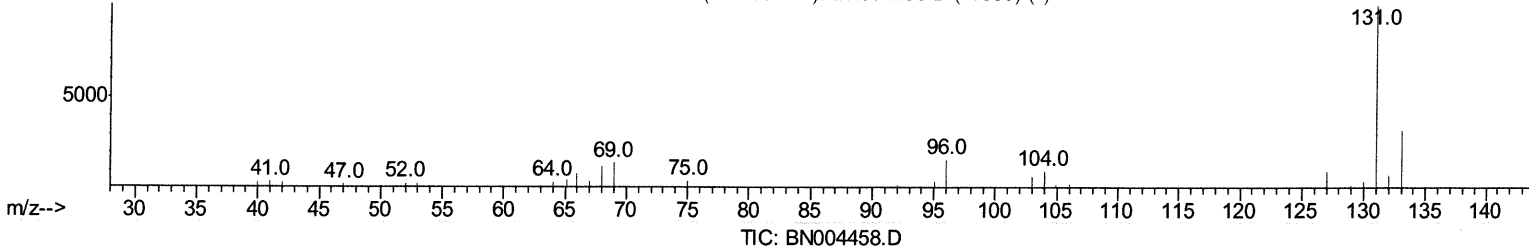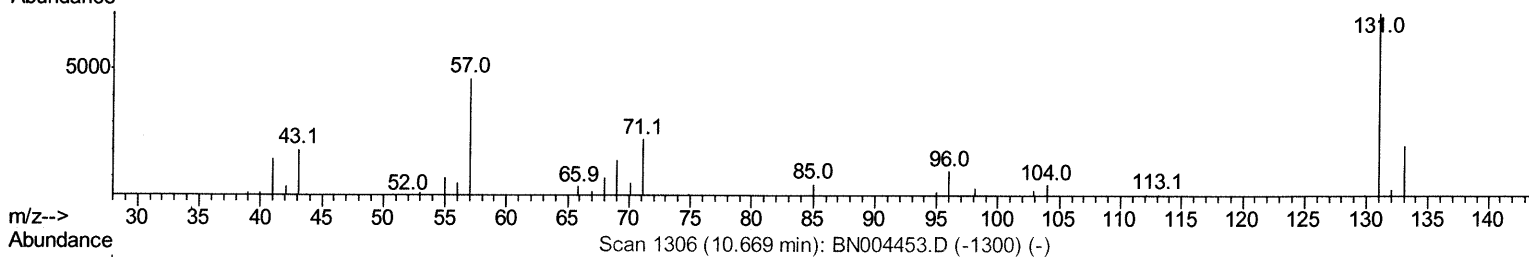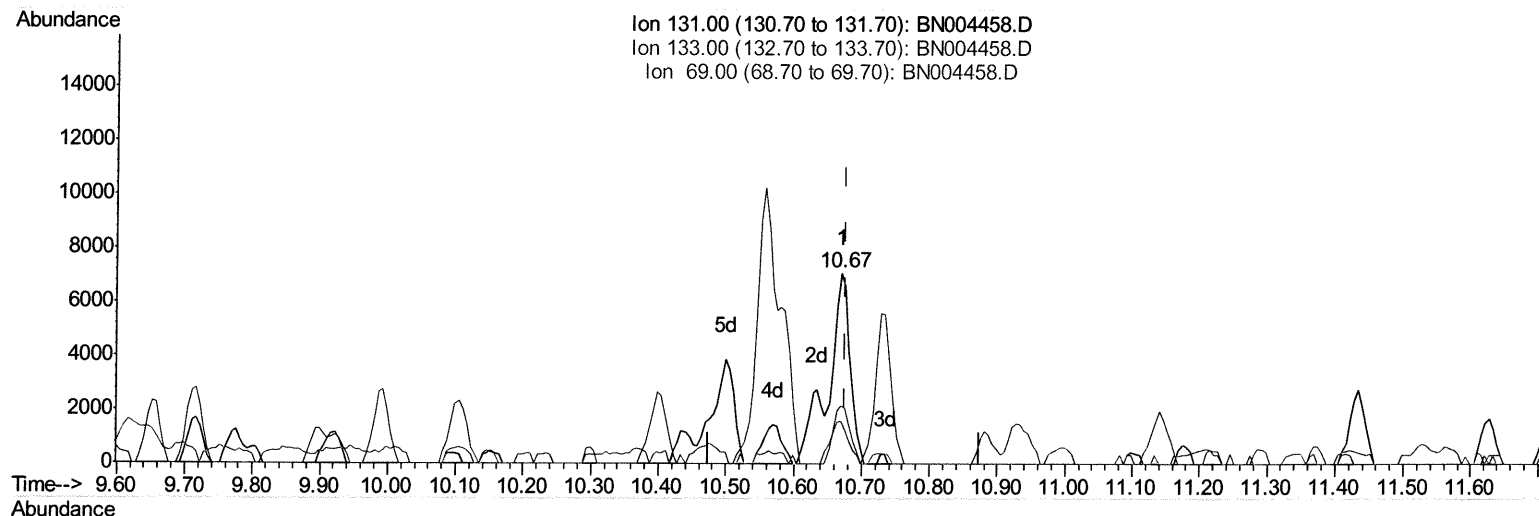

(29) 4-Chloroaniline-d4 (S)

10.669min (-0.006) 7.59ng/ul m

response 16221

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	30.27
69.00	14.90	22.62#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021919\
Data File : BN004458.D
Acq On : 19 Feb 2019 14:04
Operator : JU/SJ
Sample : K1455-01 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BE801

Manual Integrations
APPROVED

Sohil
2/20/2019 2:08:12 PM

Quant Time: Feb 19 14:56:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 19 14:16:20 2019
Response via : Initial Calibration

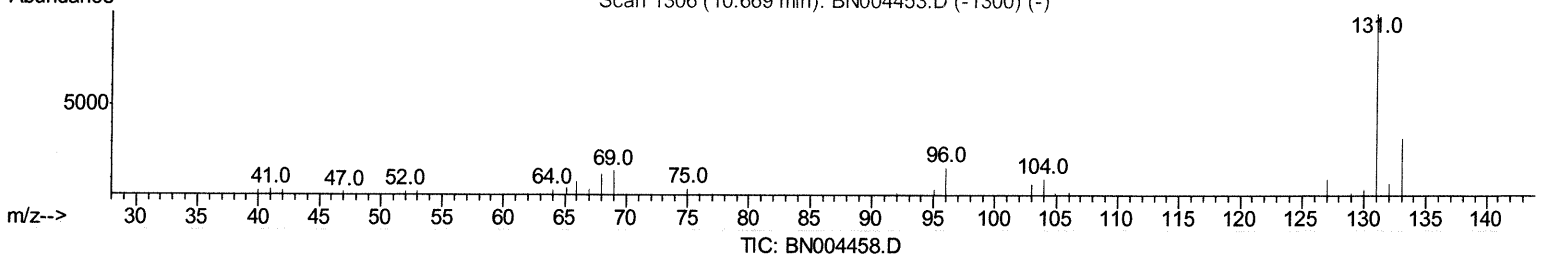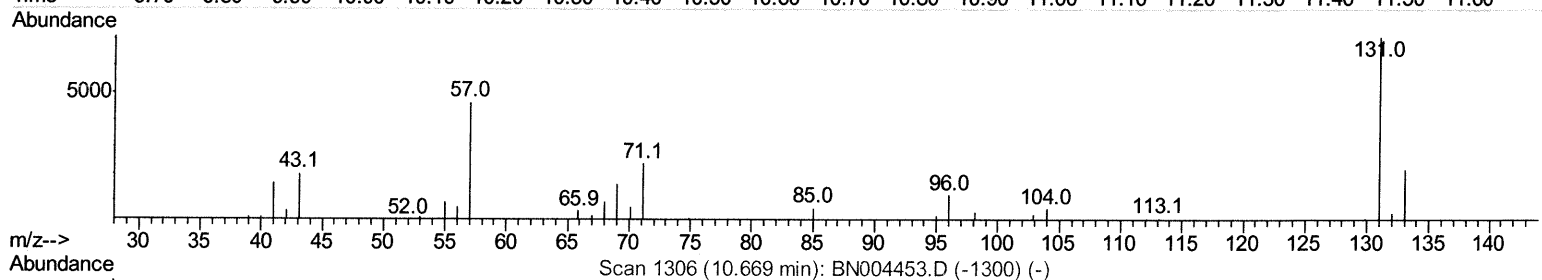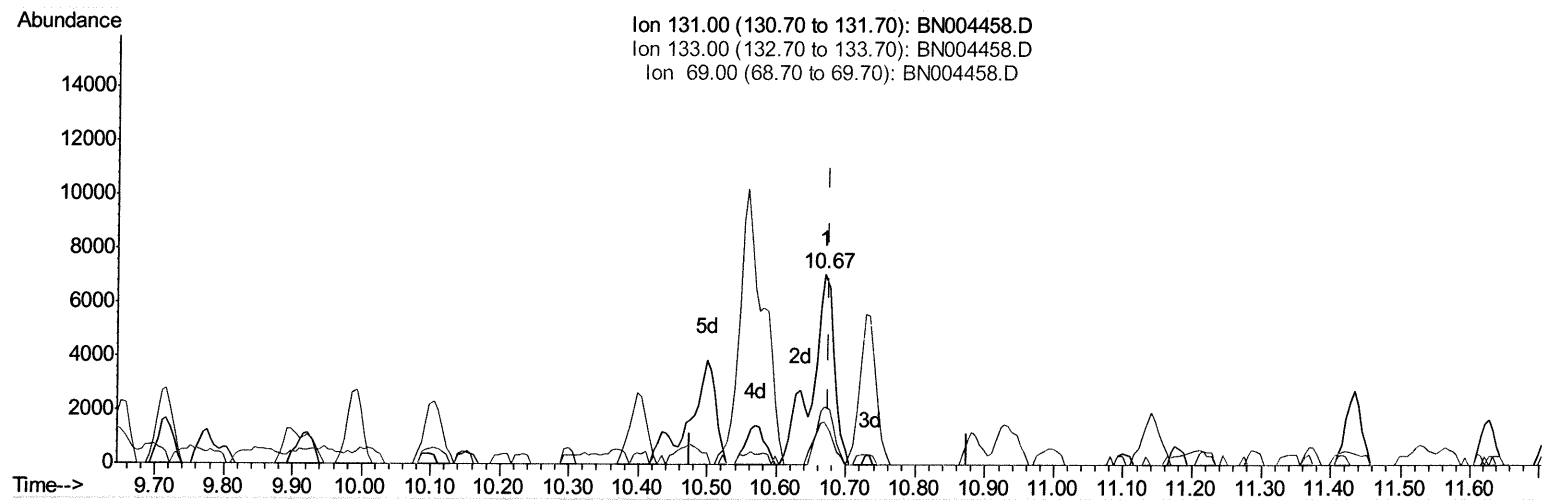

(29) 4-Chloroaniline-d4 (S)

10.669min (-0.006) 5.55ng/ul

response 11870

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	30.27
69.00	14.90	22.62#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021919\
 Data File : BN004458.D
 Acq On : 19 Feb 2019 14:04
 Operator : JU/SJ
 Sample : K1455-01 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 BE801

Manual Integrations
 APPROVED

Sohil
 2/20/2019 2:08:12 PM

Quant Time: Feb 19 15:05:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Feb 19 14:16:20 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	25585	20.00	nq/ul	0.00
18) Naphthalene-d8	10.53	136	123359	20.00	nq/ul	0.00
36) Acenaphthene-d10	14.38	164	80333	20.00	nq/ul	0.00
62) Phenanthrene-d10	17.13	188	195520	20.00	nq/ul	0.00
78) Chrysene-d12	21.33	240	278191	20.00	nq/ul	0.00
86) Perylene-d12	23.61	264	353229	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	nq/uL	
5) Phenol-d5	6.90	99	9126	4.00	nq/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	4803	4.20	nq/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	7821	4.23	nq/ul	0.00
13) 4-Methylphenol-d8	8.43	113	8073	4.12	nq/ul	0.00
19) Nitrobenzene-d5	8.90	128	3922	4.80	nq/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	3521	4.13	nq/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	8686	4.49	nq/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	16221m	7.59	nq/ul	0.00
44) Dimethylphthalate-d6	13.79	166	33731	4.95	nq/ul	0.00
47) Acenaphthylene-d8	14.07	160	41090	5.09	nq/ul	0.00
52) 4-Nitrophenol-d4	14.57	143	2464	1.89	nq/ul	0.00
58) Fluorene-d10	15.37	176	35216	5.87	nq/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	1256	1.10	nq/ul	0.00
71) Anthracene-d10	17.23	188	53955	5.76	nq/ul	0.00
79) Pyrene-d10	19.53	212	65870	5.28	nq/ul	0.00
90) Benzo(a)pyrene-d12	23.46	264	100446	5.42	ng/ul	0.00

Target Compounds

				Ovalue	
28) Naphthalene	10.58	128	68607	10.787	nq/ul 98
34) 2-Methylnaphthalene	12.19	142	9862	2.021	nq/ul 100
35) 1-Methylnaphthalene	12.41	142	8504	1.768	nq/ul# 96
59) Fluorene	15.43	166	7805	1.206	nq/ul# 93
70) Phenanthrene	17.17	178	60365	5.565	nq/ul 98
72) Anthracene	17.26	178	556158	50.923	nq/ul 100
73) 1,2,3,4-Tetrachlorobenzene	13.17	216	8768	3.269	nq/uL 98
76) Di-n-butylphthalate	18.09	149	22042	2.058	nq/ul# 95
77) Fluoranthene	19.19	202	109483	8.198	nq/ul 99
80) Pyrene	19.56	202	95087	6.181	nq/ul 98
83) Benzo(a)anthracene	21.32	228	58482	3.411	nq/ul# 93
84) Bis(2-ethylhexyl)phthalate	21.24	149	250953	31.671	nq/ul 100
85) Chrysene	21.37	228	66083	4.060	nq/ul# 95
87) Di-n-octyl phthalate	22.13	149	40655	2.404	nq/ul 100
88) Benzo(b)fluoranthene	22.92	252	90050	4.305	nq/ul# 88
89) Benzo(k)fluoranthene	22.96	252	28844	1.418	nq/ul# 81
91) Benzo(a)pyrene	23.50	252	43937	2.152	nq/ul# 84
92) Indeno(1,2,3-cd)pyrene	25.89	276	40196	1.551	nq/ul 95
94) Benzo(g,h,i)perylene	26.60	276	36299	1.671	nq/ul 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed