


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021919\
Data File : BN004452.D
Acq On : 19 Feb 2019 10:14
Operator : JU/SJ
Sample : DFTPP05
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTD02075

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION
Last Update : Thu Feb 14 07:13:45 2019

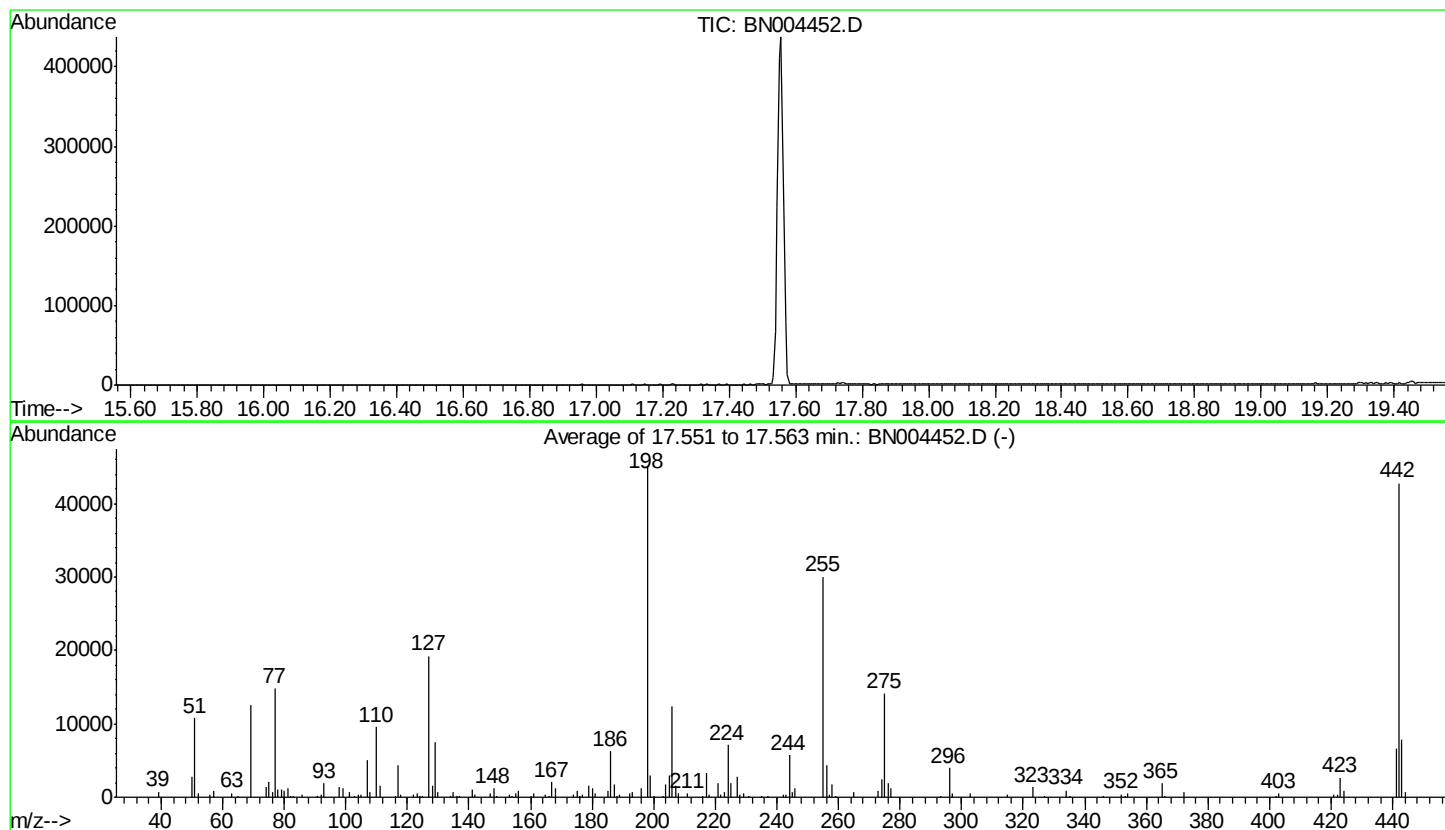

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	10786	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.8	12553	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	19248	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45184	PASS
199	198	5	9	6.7	3047	PASS
275	198	10	60	31.1	14049	PASS
365	198	1	100	4.1	1841	PASS
441	198	0.01	100	14.9	6711	PASS
442	198	50	100	94.7	42797	PASS
443	442	15	24	18.4	7857	PASS

m/z	Abundance
39.00	993.0
43.90	311.0
50.00	3649.0
51.00	13714.0
52.00	747.0
55.90	454.0
57.00	1047.0
63.00	635.0
65.00	307.0
69.00	15968.0
74.00	1702.0
75.00	2644.0
76.00	880.0
77.00	18432.0
78.00	1285.0
79.00	1209.0
80.00	1066.0
81.00	1407.0
81.90	313.0
83.00	323.0
85.90	441.0
91.00	348.0
92.00	456.0
93.00	2239.0
98.00	1744.0
99.00	1552.0
101.00	762.0
103.00	305.0
104.00	496.0
104.90	570.0
107.00	5992.0
107.90	935.0
110.00	11638.0
111.00	1853.0
116.00	384.0
117.00	5506.0
117.90	461.0
121.90	455.0
123.00	678.0
123.90	307.0
125.00	315.0
127.00	22936.0
128.00	1782.0
129.00	8943.0
130.00	836.0
135.00	801.0
135.90	325.0
137.00	402.0
140.90	1265.0
141.90	450.0
147.00	649.0
148.00	1371.0
149.00	391.0
152.90	432.0
155.00	615.0
156.00	1053.0
160.00	389.0
161.00	641.0
164.90	489.0
166.00	360.0
167.00	2522.0
168.00	1593.0
174.00	514.0
175.00	1019.0
176.00	309.0
176.90	488.0
179.00	1789.0
180.00	1419.0
181.00	603.0
185.00	1036.0
186.00	7041.0
187.00	2190.0
188.00	372.0
188.90	489.0
192.00	641.0
193.00	696.0
196.00	1510.0
198.00	50432.0
199.00	3404.0
199.90	309.0
203.10	373.0
204.00	2002.0
205.00	3192.0
206.00	13936.0
207.00	2274.0
208.00	615.0
210.90	469.0
217.00	3692.0
218.00	501.0
221.00	2331.0
221.90	507.0

Instrument :
BNA_N
LabSampleId :
SSTD02075

223.00	845.0
224.00	7858.0
225.00	2161.0
227.00	3038.0
228.00	483.0
229.00	691.0
237.00	384.0
242.00	388.0
243.00	440.0
244.00	6183.0
245.00	814.0
246.00	1295.0
255.00	31944.0
256.00	4985.0
257.00	429.0
257.90	1840.0
265.00	709.0
273.00	959.0
274.00	2590.0
275.00	14996.0
276.00	2043.0
277.00	1243.0
296.00	4011.0
296.90	648.0
303.00	528.0
315.00	443.0
323.00	1224.0
334.00	928.0
352.00	309.0
353.00	364.0
354.00	434.0
365.00	1813.0
372.00	690.0
403.00	399.0
421.00	304.0
422.00	368.0
423.00	2381.0
424.00	718.0
441.10	6057.0
442.00	38112.0
443.00	7105.0
444.00	779.0

Instrument :
BNA_N
LabSampleId :
SSTD02075

m/z	Abundance
39.00	877.0
44.00	310.0
50.00	2996.0
51.00	12410.0
52.00	723.0
55.90	426.0
57.00	1023.0
63.00	693.0
69.00	14084.0
74.00	1569.0
75.00	2424.0
76.00	897.0
77.00	17216.0
78.00	1135.0
79.00	1269.0
79.90	871.0
81.00	1383.0
82.00	317.0
82.90	311.0
86.00	412.0
90.90	331.0
92.00	355.0
93.00	2212.0
98.00	1756.0
99.00	1495.0
101.00	824.0
104.00	465.0
105.00	506.0
107.00	6007.0
108.00	901.0
110.00	10947.0
111.00	1754.0
115.90	380.0
117.00	5195.0
118.00	452.0
122.00	392.0
123.00	683.0
123.90	306.0
127.00	22608.0
128.00	1808.0
129.00	8645.0
130.00	800.0
134.00	307.0
135.00	698.0
137.00	401.0
141.00	1236.0
142.00	360.0
147.00	643.0
148.00	1341.0
149.00	319.0
152.90	427.0
153.90	336.0
155.00	708.0
156.00	1196.0
160.00	371.0
161.00	612.0
164.90	444.0
165.90	420.0
167.00	2271.0
168.00	1422.0
174.00	528.0
175.00	982.0
177.00	470.0
179.00	2027.0
179.90	1346.0
180.90	640.0
185.00	951.0
186.00	7347.0
187.00	2064.0
188.90	477.0
192.00	638.0
193.00	756.0
196.00	1435.0
198.00	53576.0
199.00	3669.0
199.90	333.0
203.00	360.0
204.00	1924.0
205.00	3366.0
206.00	14233.0
207.00	2486.0
208.00	599.0
211.00	551.0
216.00	398.0
217.00	4031.0
218.00	515.0
221.00	2324.0
223.00	919.0
224.00	8310.0
225.00	2233.0
227.00	3405.0

Instrument :
BNA_N
LabSampleId :
SSTD02075

227.90	538.0
229.00	733.0
231.00	314.0
234.90	323.0
237.00	354.0
242.00	425.0
243.00	441.0
244.00	6754.0
245.00	909.0
246.00	1304.0
255.00	35280.0
256.00	5082.0
256.90	428.0
258.00	1935.0
258.90	324.0
265.00	936.0
272.90	951.0
274.00	2949.0
275.00	16576.0
276.00	2351.0
277.00	1357.0
293.00	314.0
296.00	4663.0
296.90	670.0
303.00	520.0
314.90	469.0
323.00	1624.0
326.90	320.0
334.00	1146.0
335.00	314.0
345.90	330.0
351.90	494.0
353.00	326.0
354.00	612.0
365.00	2176.0
365.90	370.0
372.00	894.0
402.00	340.0
403.00	510.0
421.00	420.0
422.00	422.0
423.00	3175.0
424.00	957.0
441.00	8092.0
442.00	51352.0
443.00	9378.0
444.00	941.0

Instrument :
BNA_N
LabSampleId :
SSTD02075

m/z	Abundance
39.00	418.0
50.00	1674.0
51.00	6234.0
57.00	450.0
63.00	363.0
69.00	7608.0
74.00	942.0
75.00	1270.0
76.00	489.0
77.00	8822.0
78.00	586.0
79.00	667.0
79.90	453.0
81.00	697.0
93.00	1118.0
97.90	939.0
98.90	751.0
101.00	398.0
103.90	309.0
107.00	3342.0
107.90	505.0
110.00	6040.0
111.00	935.0
117.00	2625.0
123.00	336.0
127.00	12202.0
128.00	961.0
129.00	4764.0
129.90	377.0
134.90	437.0
140.90	657.0
147.00	384.0
147.90	760.0
154.90	391.0
156.00	643.0
160.90	316.0
167.00	1390.0
168.00	842.0
175.00	636.0
179.00	1065.0
180.00	772.0
180.90	302.0
185.00	578.0
186.00	4426.0
187.00	1238.0
192.00	413.0
192.90	441.0
195.90	841.0
198.00	31544.0
199.00	2070.0
204.00	1088.0
205.00	2142.0
206.10	8796.0
207.00	1524.0
208.00	411.0
210.90	356.0
217.00	2421.0
221.00	1255.0
221.80	317.0
222.90	550.0
224.00	5281.0
225.00	1231.0
227.00	2146.0
228.90	407.0
244.00	4196.0
245.00	490.0
246.00	899.0
255.00	22848.0
256.00	3254.0
257.00	304.0
258.00	1253.0
265.00	548.0
273.00	663.0
274.00	1802.0
275.00	10576.0
276.00	1500.0
277.00	827.0
296.00	3222.0
296.90	425.0
302.90	387.0
314.90	340.0
323.00	1165.0
334.00	741.0
352.00	361.0
354.00	422.0
364.90	1535.0
372.00	537.0
403.00	420.0
421.00	315.0
422.00	368.0
423.00	2336.0

Instrument :
BNA_N
LabSampleId :
SSTD02075

424.00	797.0
441.10	5984.0
442.00	38928.0
443.00	7089.0
443.90	604.0

Instrument :
BNA_N
LabSampleId :
SSTD02075

Scan 2471 (17.522 min): BN004452.D
DFTPP05

m/z	Abundance
44.00	335.0
207.00	544.0

Instrument :

BNA_N

LabSampleId :

SSTD02075