


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022020\
 Data File : BN009787.D
 Acq On : 20 Feb 2020 19:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 19 15:57:43 2020

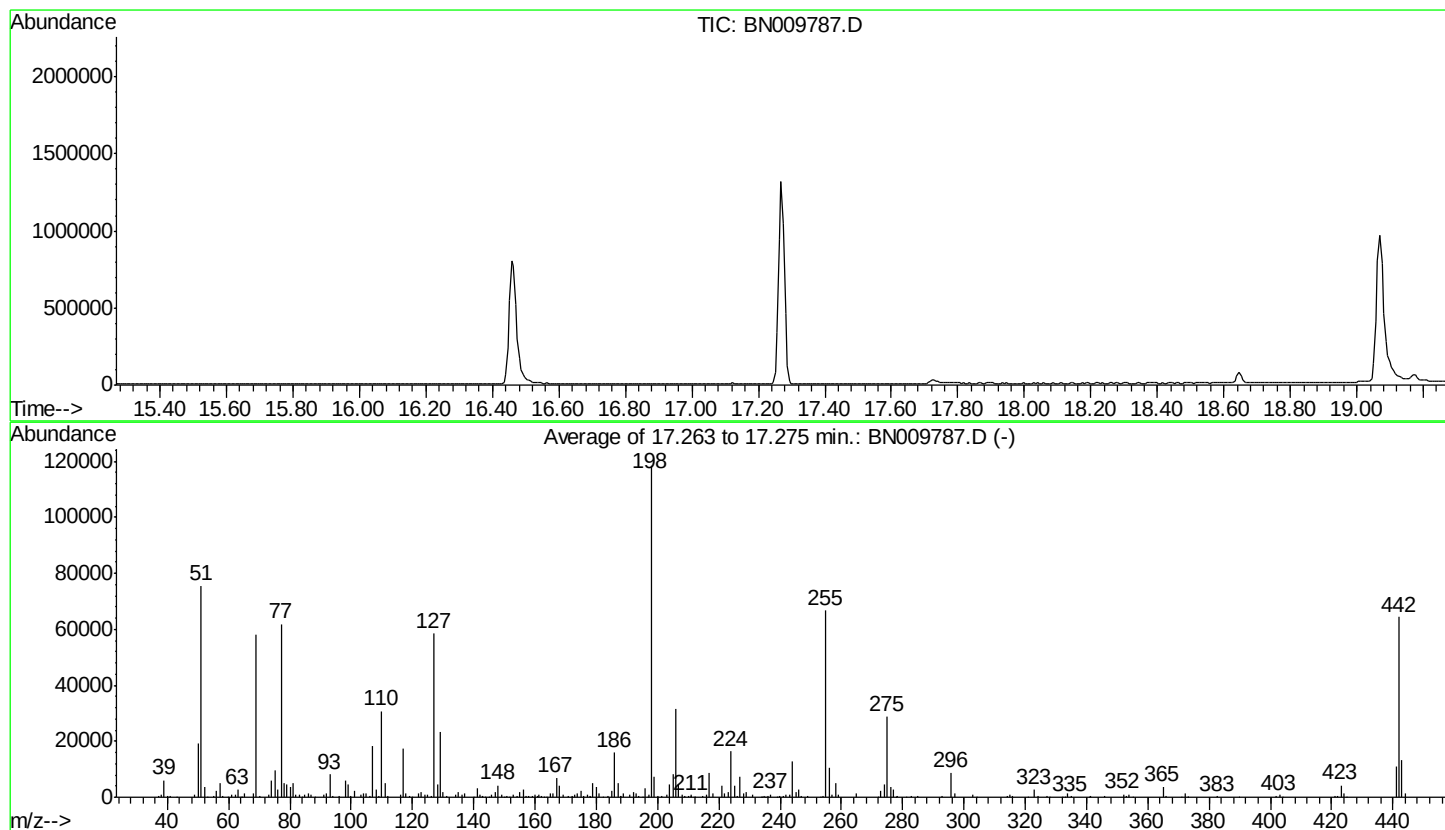

AutoFind: Scans 2427, 2428, 2429; Background Corrected with Scan 2421

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.7	75490	PASS
68	69	0.00	2	2.0	1168	PASS
69	198	0.00	100	49.1	58213	PASS
70	69	0.00	2	0.6	343	PASS
127	198	10	80	49.4	58488	PASS
197	198	0.00	2	0.7	797	PASS
198	198	100	100	100.0	118504	PASS
199	198	5	9	6.3	7521	PASS
275	198	10	60	24.2	28677	PASS
365	198	1	100	3.1	3692	PASS
441	198	0.01	100	9.2	10927	PASS
442	198	50	100	54.4	64482	PASS
443	442	15	24	20.7	13323	PASS