


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022120\
 Data File : BN009803.D
 Acq On : 21 Feb 2020 12:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 19 15:57:43 2020

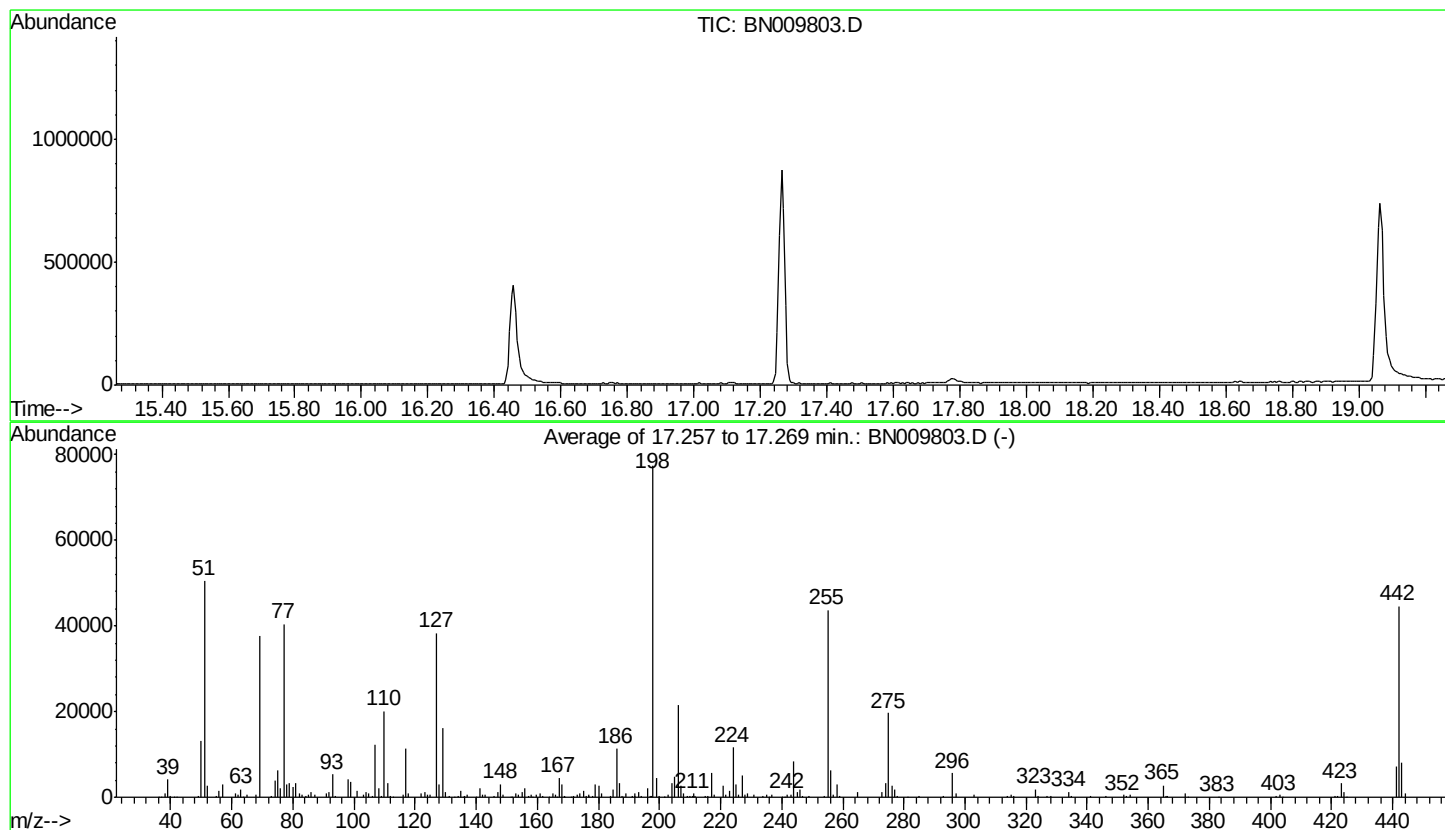

AutoFind: Scans 2426, 2427, 2428; Background Corrected with Scan 2420

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.3	50565	PASS
68	69	0.00	2	1.9	706	PASS
69	198	0.00	100	48.8	37776	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	38405	PASS
197	198	0.00	2	0.3	256	PASS
198	198	100	100	100.0	77429	PASS
199	198	5	9	5.7	4445	PASS
275	198	10	60	25.5	19708	PASS
365	198	1	100	3.6	2820	PASS
441	198	0.01	100	9.2	7132	PASS
442	198	50	100	57.6	44600	PASS
443	442	15	24	18.0	8013	PASS