


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
Data File : BN013705.D
Acq On : 21 Feb 2021 01:54
Operator : CG/JU
Sample : M1415-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBH22

Manual Integrations
APPROVED

mohammad
2/22/2021 2:13:58 PM

Quant Time: Feb 22 00:51:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 23:16:49 2021
Response via : Initial Calibration

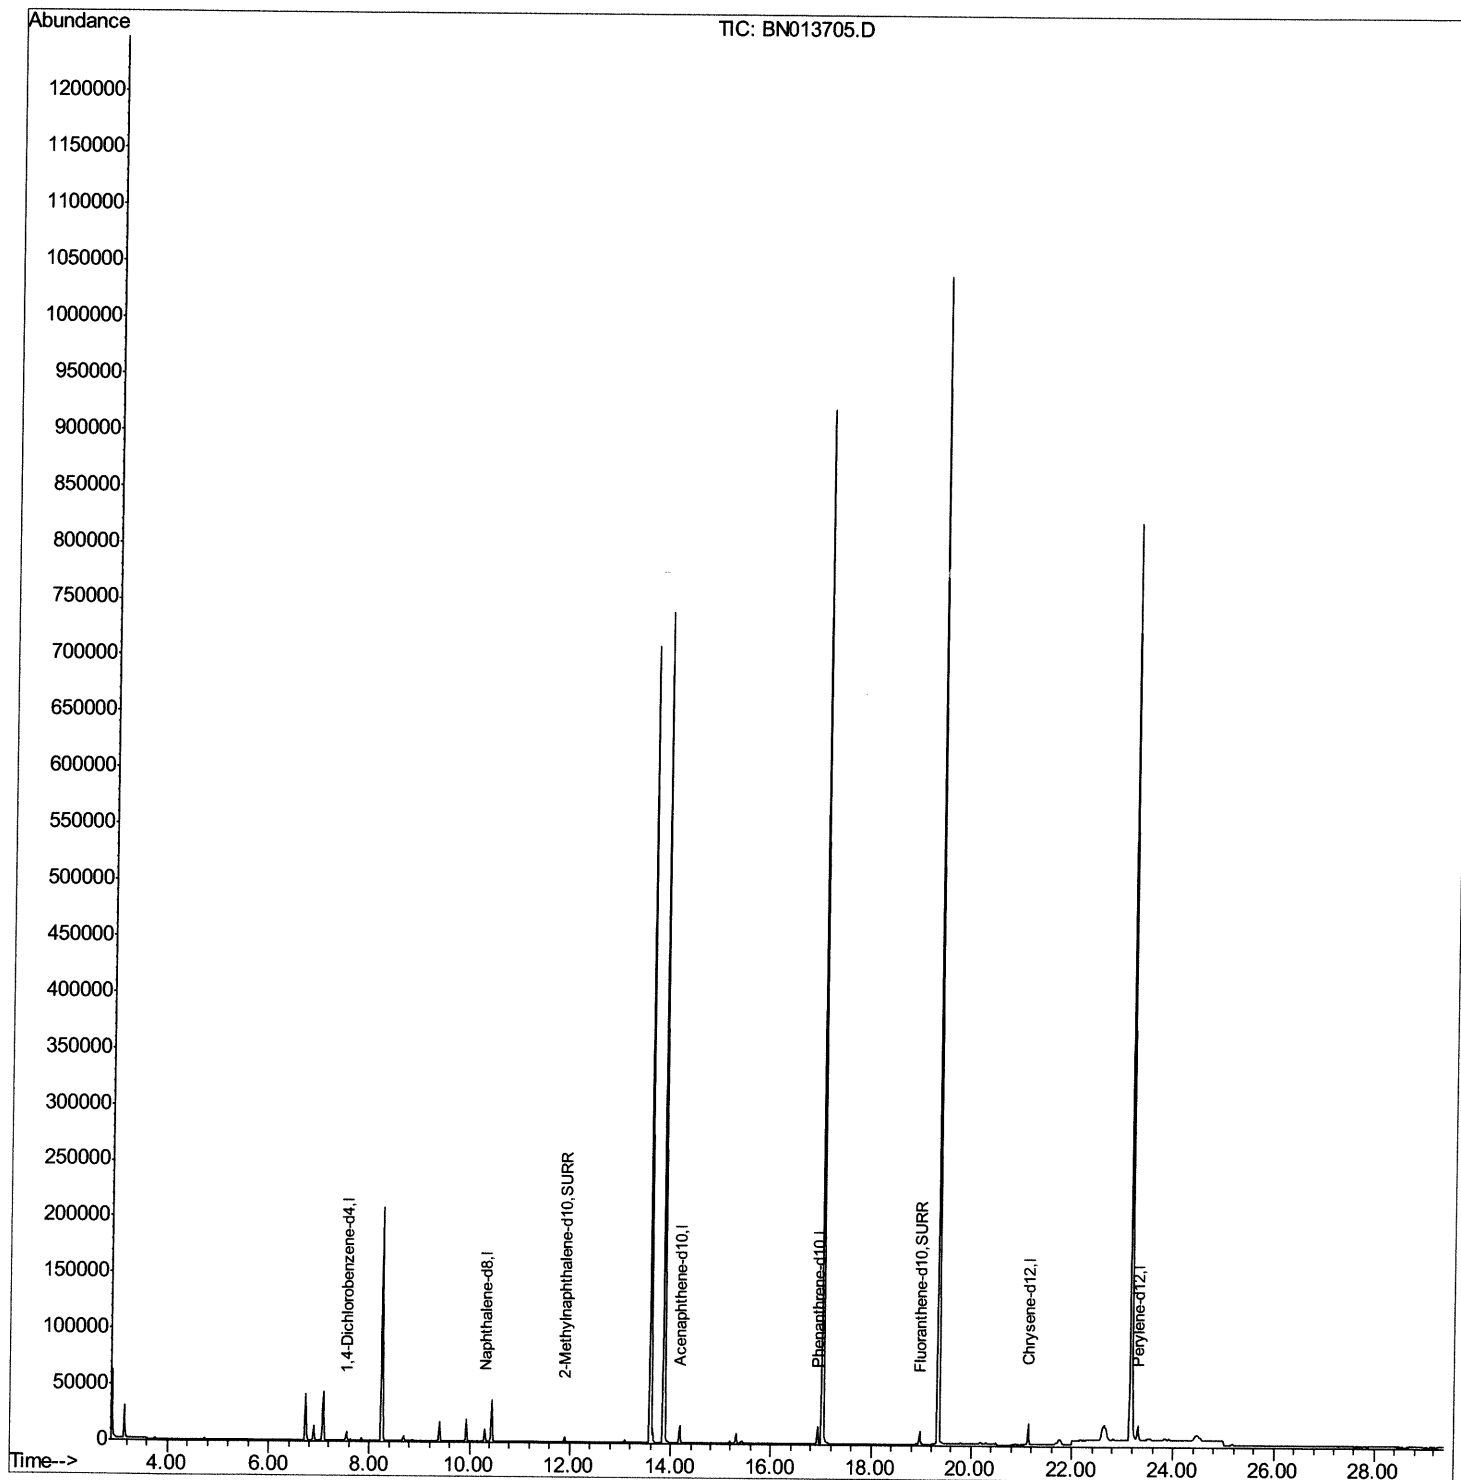

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
 Data File : BN013705.D
 Acq On : 21 Feb 2021 01:54
 Operator : CG/JU
 Sample : M1415-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 DBH22

Manual Integrations
APPROVED

mohammad
 2/22/2021 2:13:58 PM

Quant Time: Feb 22 00:48:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 20 23:16:49 2021
 Response via : Initial Calibration

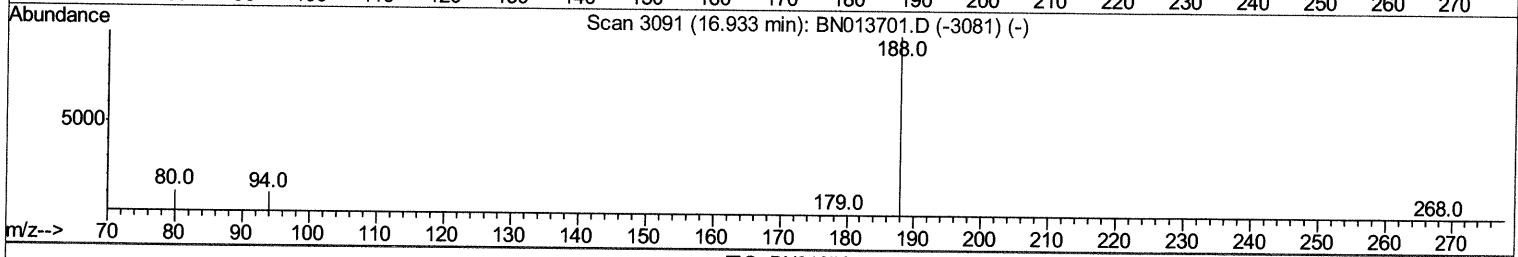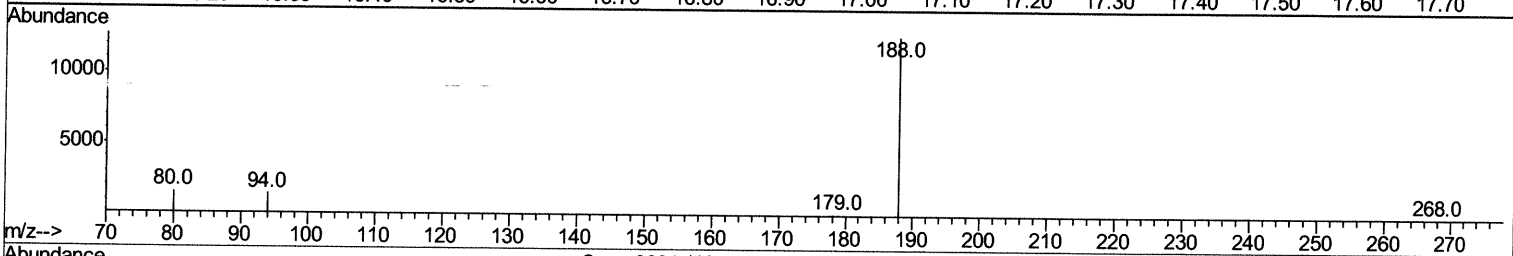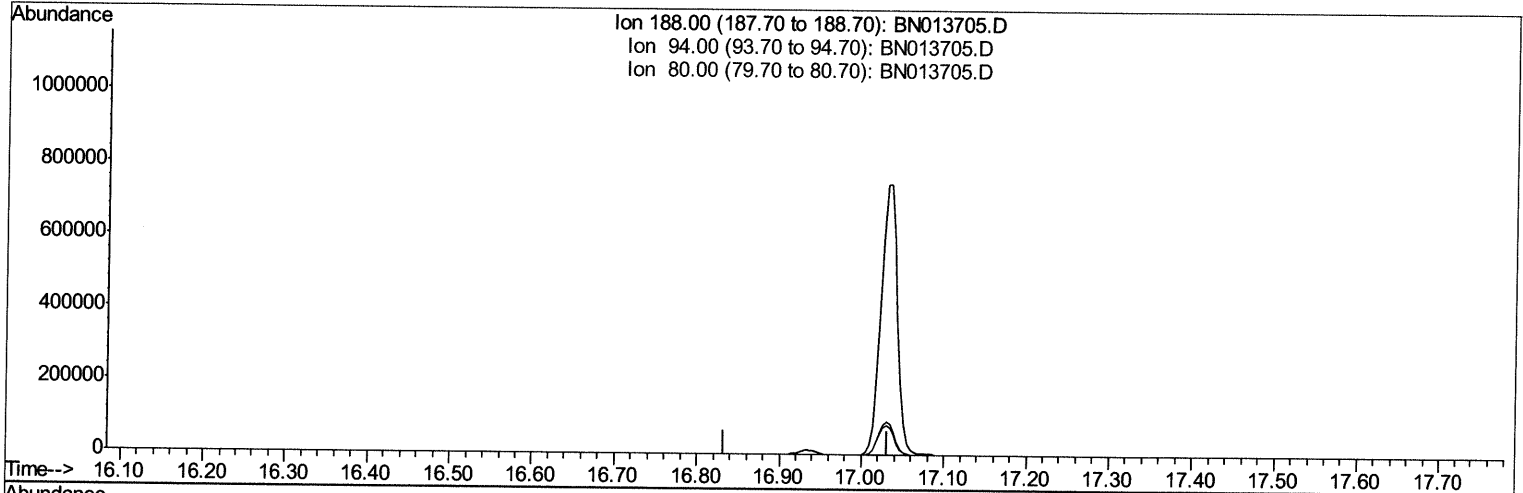

TIC: BN013705.D

(10) Phenanthrene-d10 (I)

16.933min (-16.933) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.70	0.00#
80.00	11.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
Data File : BN013705.D
Acq On : 21 Feb 2021 01:54
Operator : CG/JU
Sample : M1415-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBH22

Manual Integrations
APPROVED

mohammad
2/22/2021 2:13:58 PM

Quant Time: Feb 22 00:48:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 23:16:49 2021
Response via : Initial Calibration

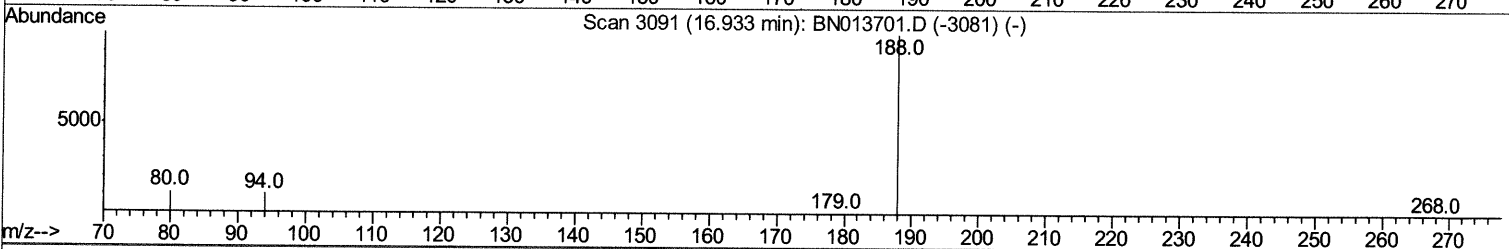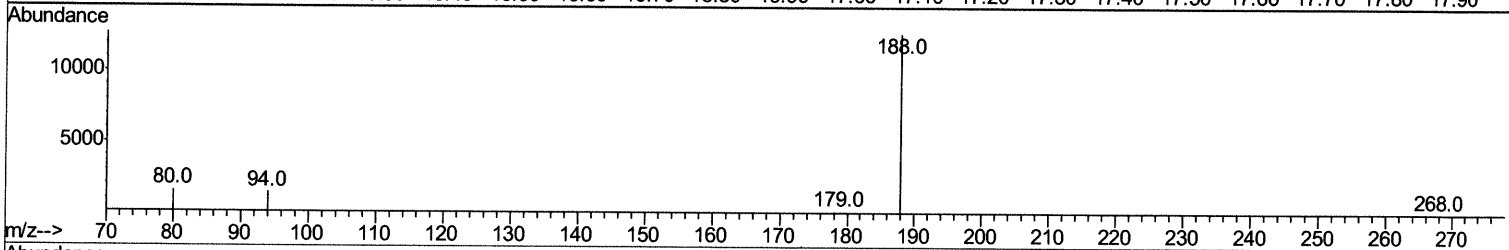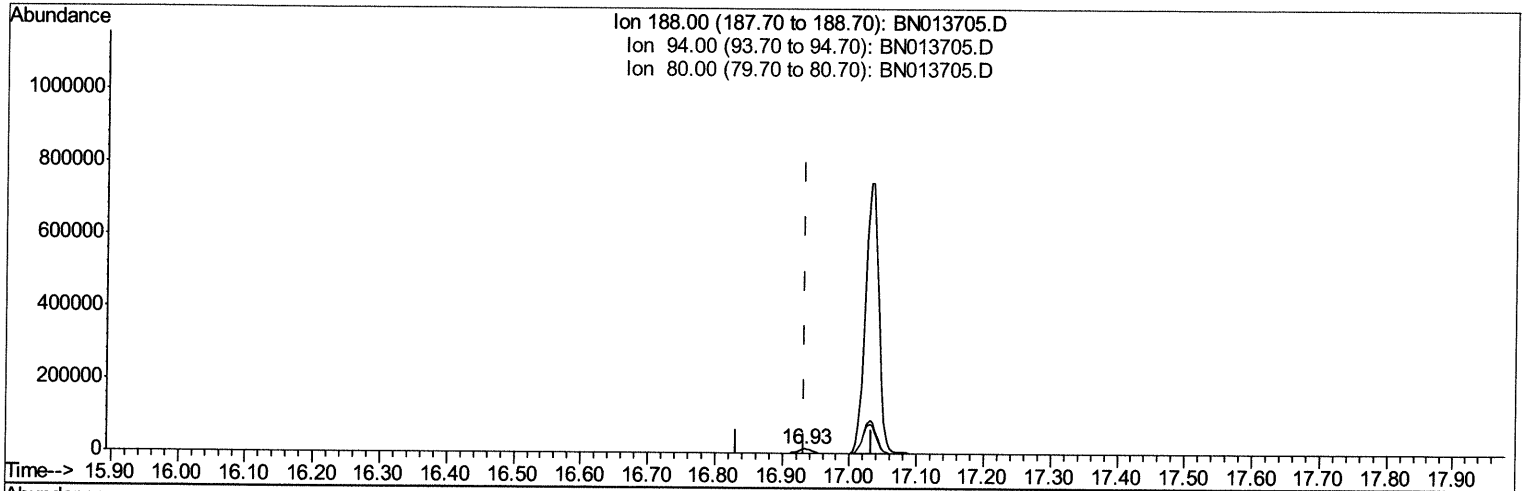

TIC: BN013705.D

(10) Phenanthrene-d10 (I)

16.933min (-0.000) 0.40ng/ul m

response 17562

Ion	Exp%	Act%
188.00	100	100
94.00	10.70	11.23
80.00	11.60	12.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
Data File : BN013705.D
Acq On : 21 Feb 2021 01:54
Operator : CG/JU
Sample : M1415-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBH22

Manual Integrations
APPROVED

mohammad
2/22/2021 2:13:58 PM

Quant Time: Feb 22 00:51:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 23:16:49 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	3674	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	14446	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	8448	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	17562m	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	16004	0.40	ng/ul	0.00
20) Perylene-d12	23.30	264	15606	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.90	152	5951	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	12808	0.27	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed