


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
Data File : BN013720.D
Acq On : 21 Feb 2021 11:29
Operator : CG/JU
Sample : M1429-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGTO

Manual Integrations
APPROVED

mohammad
2/22/2021 2:14:39 PM

Quant Time: Feb 22 01:51:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 22 01:25:38 2021
Response via : Initial Calibration

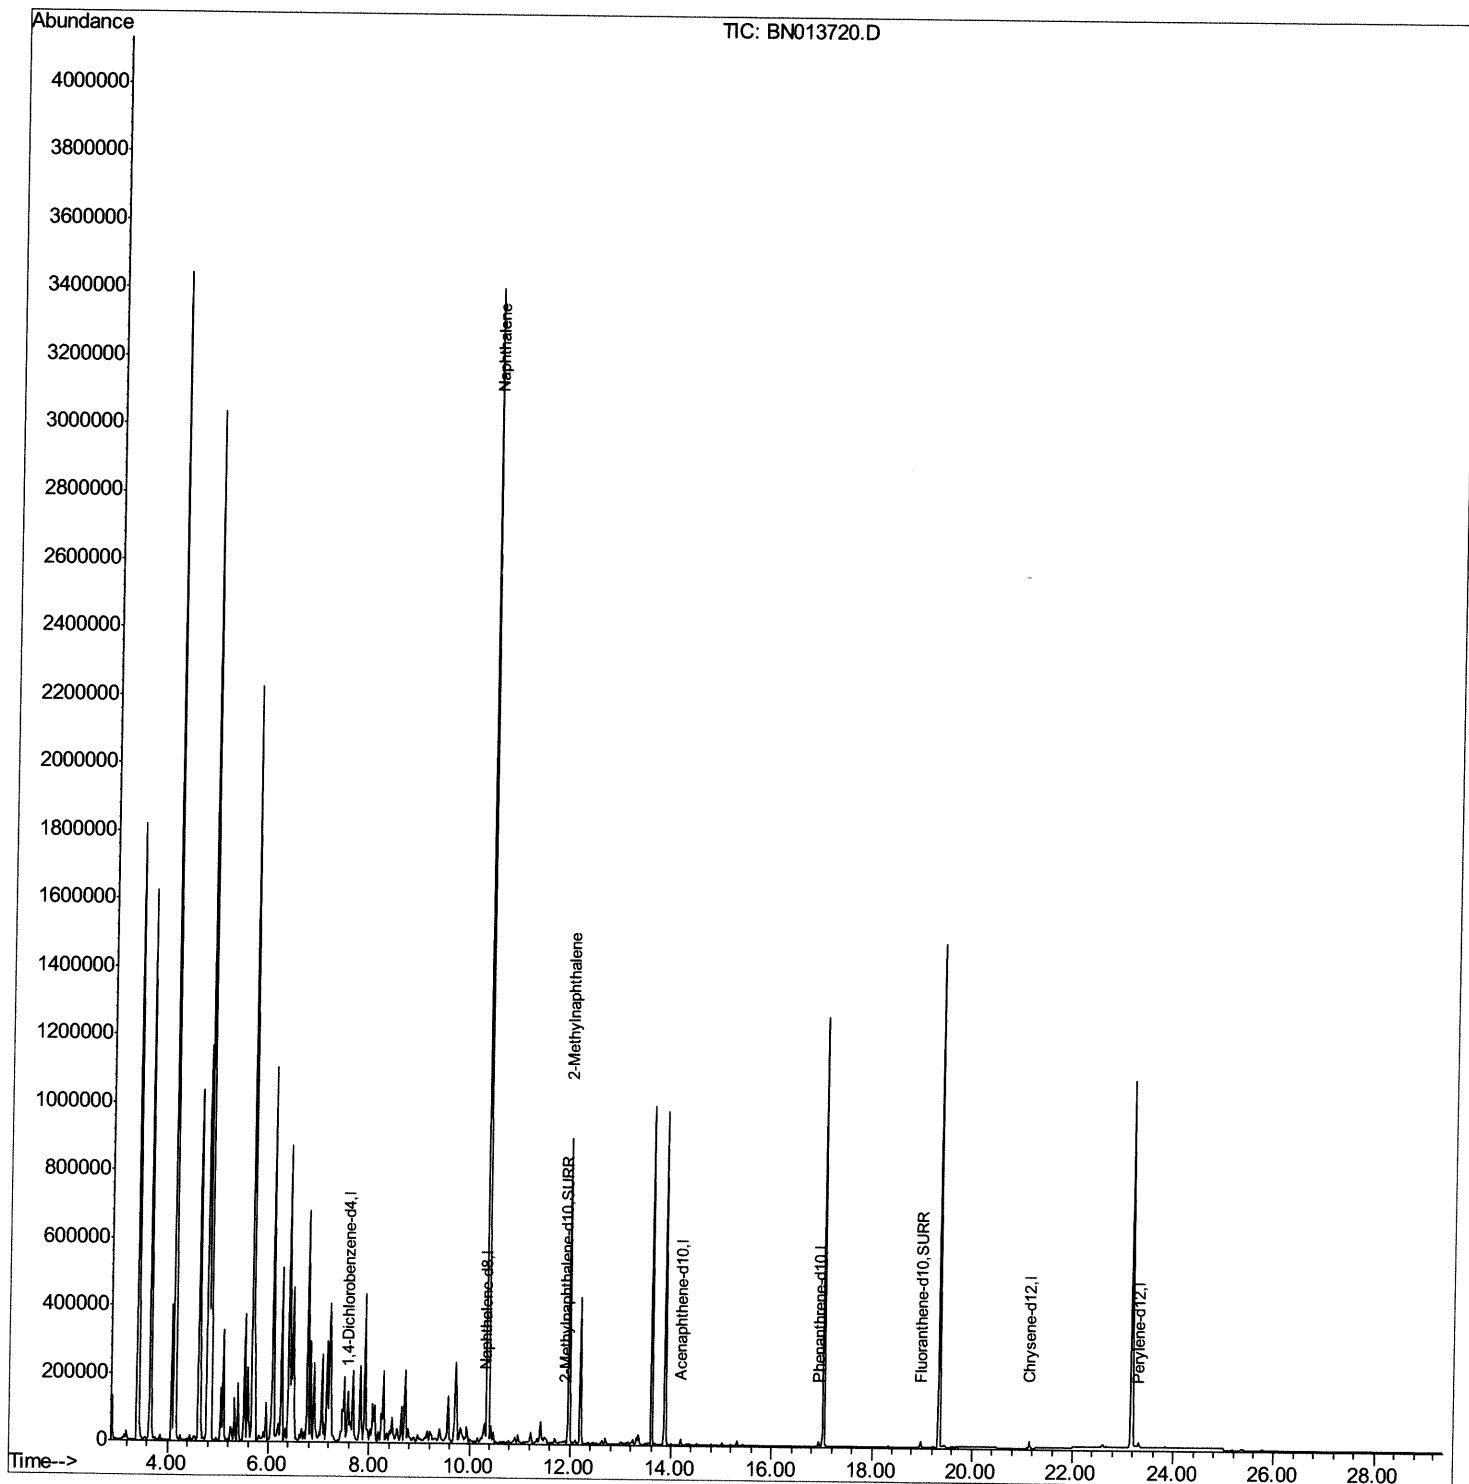

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
Data File : BN013720.D
Acq On : 21 Feb 2021 11:29
Operator : CG/JU
Sample : M1429-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGTO

Manual Integrations
APPROVED

mohammad
2/22/2021 2:14:39 PM

Quant Time: Feb 22 01:50:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 22 01:25:38 2021
Response via : Initial Calibration

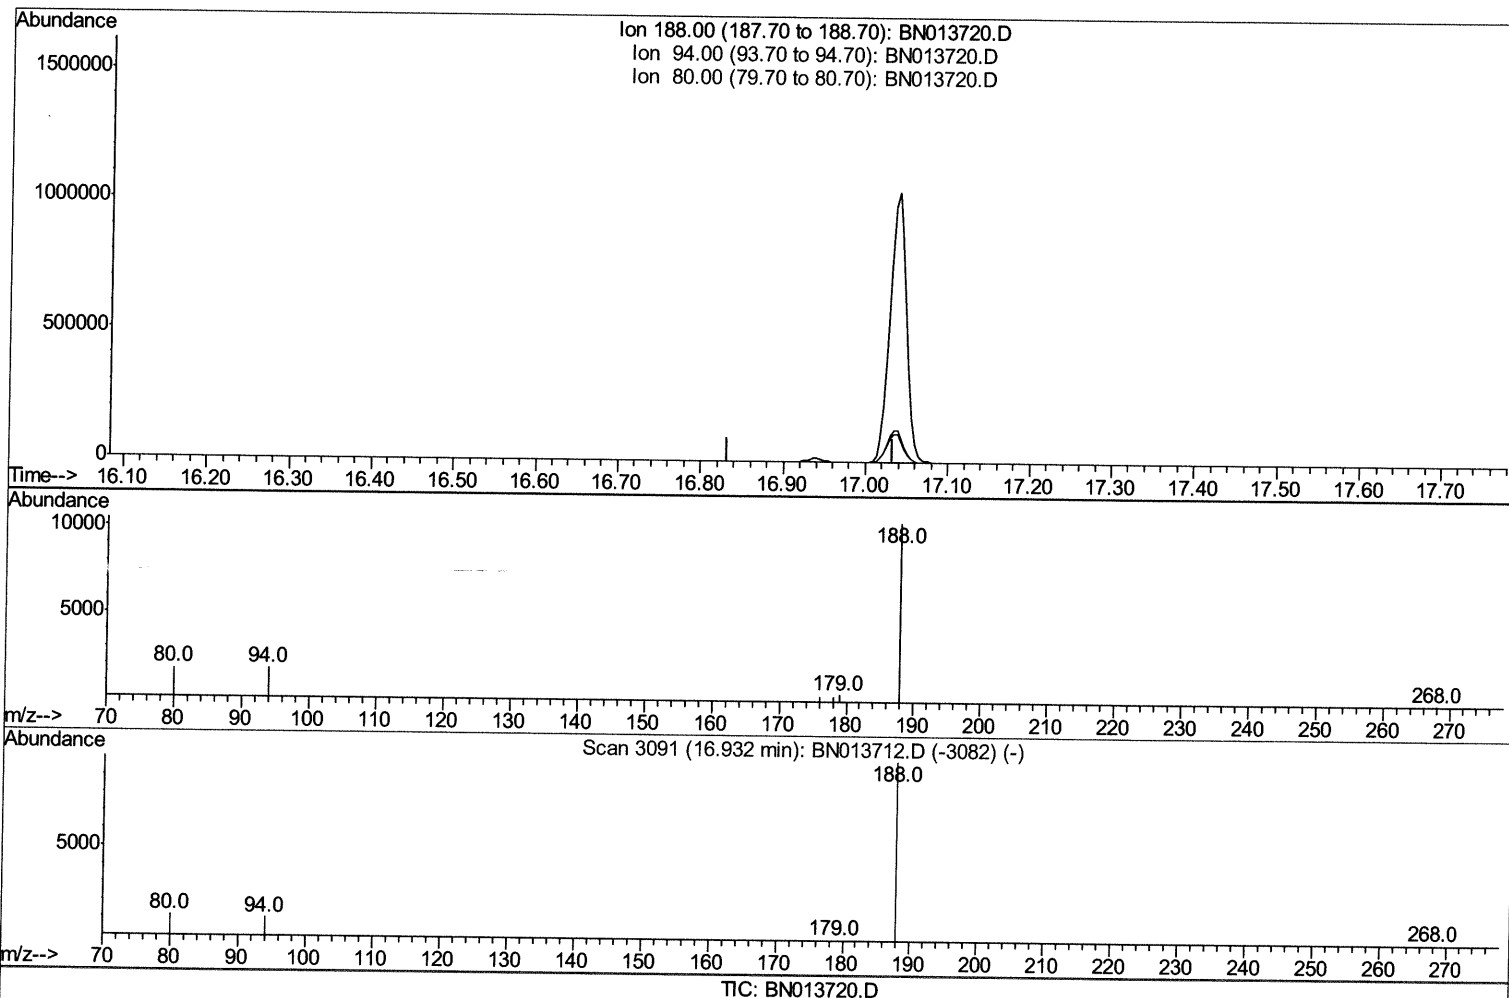

(10) Phenanthrene-d10 (I)

16.933min (-16.933) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.70	0.00#
80.00	11.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
 Data File : BN013720.D
 Acq On : 21 Feb 2021 11:29
 Operator : CG/JU
 Sample : M1429-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGTO

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:14:39 PM

Quant Time: Feb 22 01:50:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 01:25:38 2021
 Response via : Initial Calibration

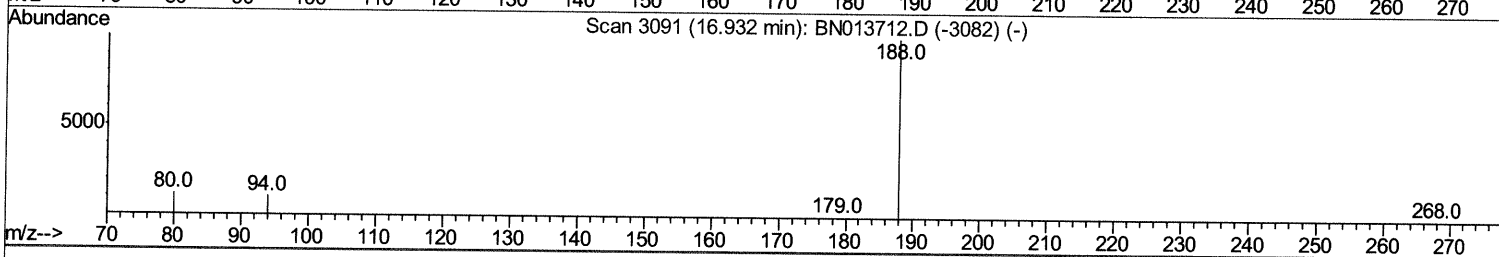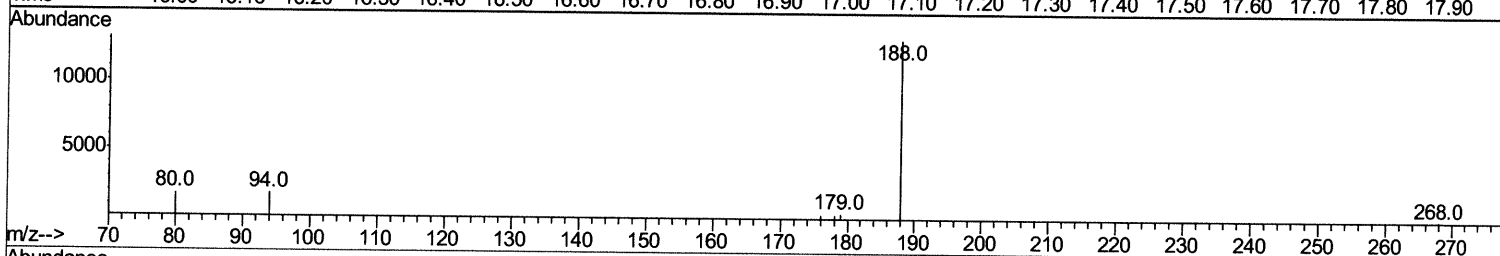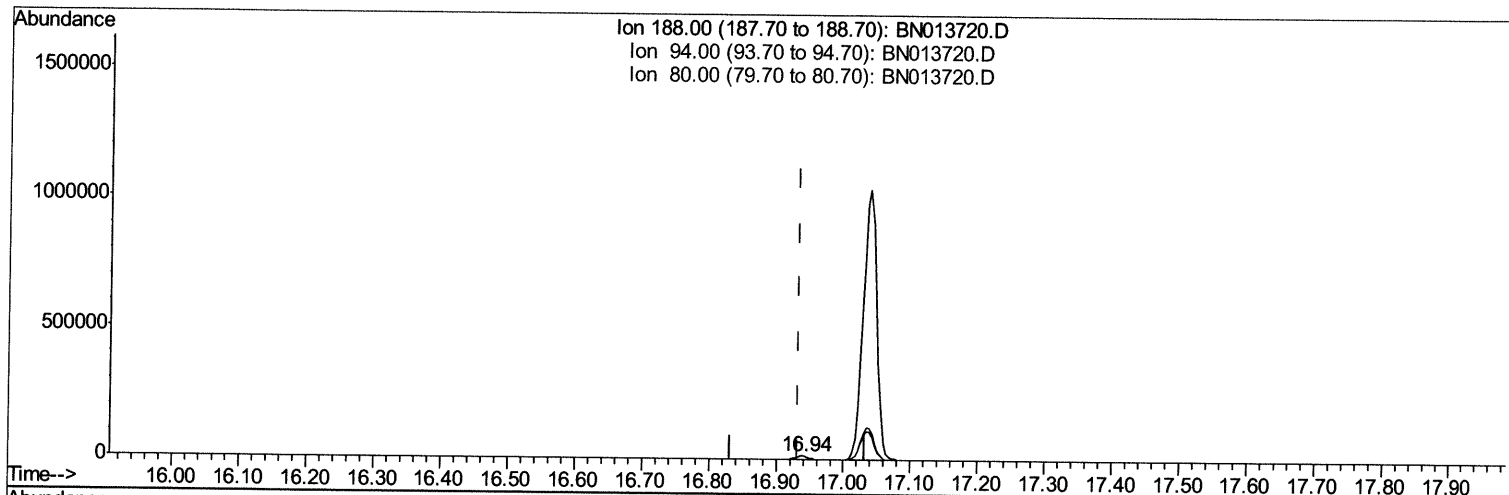

TIC: BN013720.D

(10) Phenanthrene-d10 (I)

16.941min (+0.008) 0.40ng/ul m

response 17677

Ion	Exp%	Act%
188.00	100	100
94.00	10.70	13.46#
80.00	11.60	13.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022121\
 Data File : BN013720.D
 Acq On : 21 Feb 2021 11:29
 Operator : CG/JU
 Sample : M1429-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGTO

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:14:39 PM

Quant Time: Feb 22 01:51:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN022121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 01:25:38 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	3413	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	14325	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	9633	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	17677m	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	15496	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	14832	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.91	152	8412	0.40	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	19005	0.40	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.36	128	4722918	125.023	ng/ul	100
5) 2-Methylnaphthalene	11.98	142	634575	24.708	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed