

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022220\
 Data File : BN009836.D
 Acq On : 22 Feb 2020 08:49
 Operator : CG/JU
 Sample : L1535-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Feb 24 00:22:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 04:46:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	123383	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.13	136	535984	20.00	ng/ul	-0.03
36) Acenaphthene-d10	14.03	164	331666	20.00	ng/ul	-0.02
62) Phenanthrene-d10	16.79	188	708607	20.00	ng/ul	-0.02
78) Chrysene-d12	21.00	240	606732	20.00	ng/ul	-0.02
86) Perylene-d12	23.10	264	653712	20.00	ng/ul	-0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	21084	7.03	ng/uL	-0.02
5) Phenol-d5	6.59	99	374295	35.66	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	6.75	67	272123	37.57	ng/ul	-0.02
9) 2-Chlorophenol-d4	6.93	132	295363	37.38	ng/ul	-0.02
13) 4-Methylphenol-d8	8.10	113	305491	36.59	ng/ul	-0.02
19) Nitrobenzene-d5	8.53	128	143829	36.68	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.25	143	164345	38.31	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	9.78	165	287917	34.91	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.29	131	407108	43.94	ng/ul	-0.03
44) Dimethylphthalate-d6	13.46	166	895163	36.13	ng/ul	-0.02
47) Acenaphthylene-d8	13.72	160	1111550	38.10	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.27	143	133874	29.59	ng/ul	-0.02
58) Fluorene-d10	15.03	176	783541	36.63	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.19	200	120791	27.44	ng/ul	-0.02
71) Anthracene-d10	16.89	188	1180297	36.34	ng/ul	-0.02
79) Pyrene-d10	19.19	212	1267664	39.97	ng/ul	-0.02
90) Benzo(a)pyrene-d12	22.97	264	1220774	37.40	ng/ul	-0.03

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.10	70	8975	1.263	ng/ul#	1
45) Dimethylphthalate	13.50	163	61454	2.377	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022220\
Data File : BN009836.D
Acq On : 22 Feb 2020 08:49
Operator : CG/JU
Sample : L1535-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Feb 24 00:22:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 04:46:48 2020
Response via : Initial Calibration

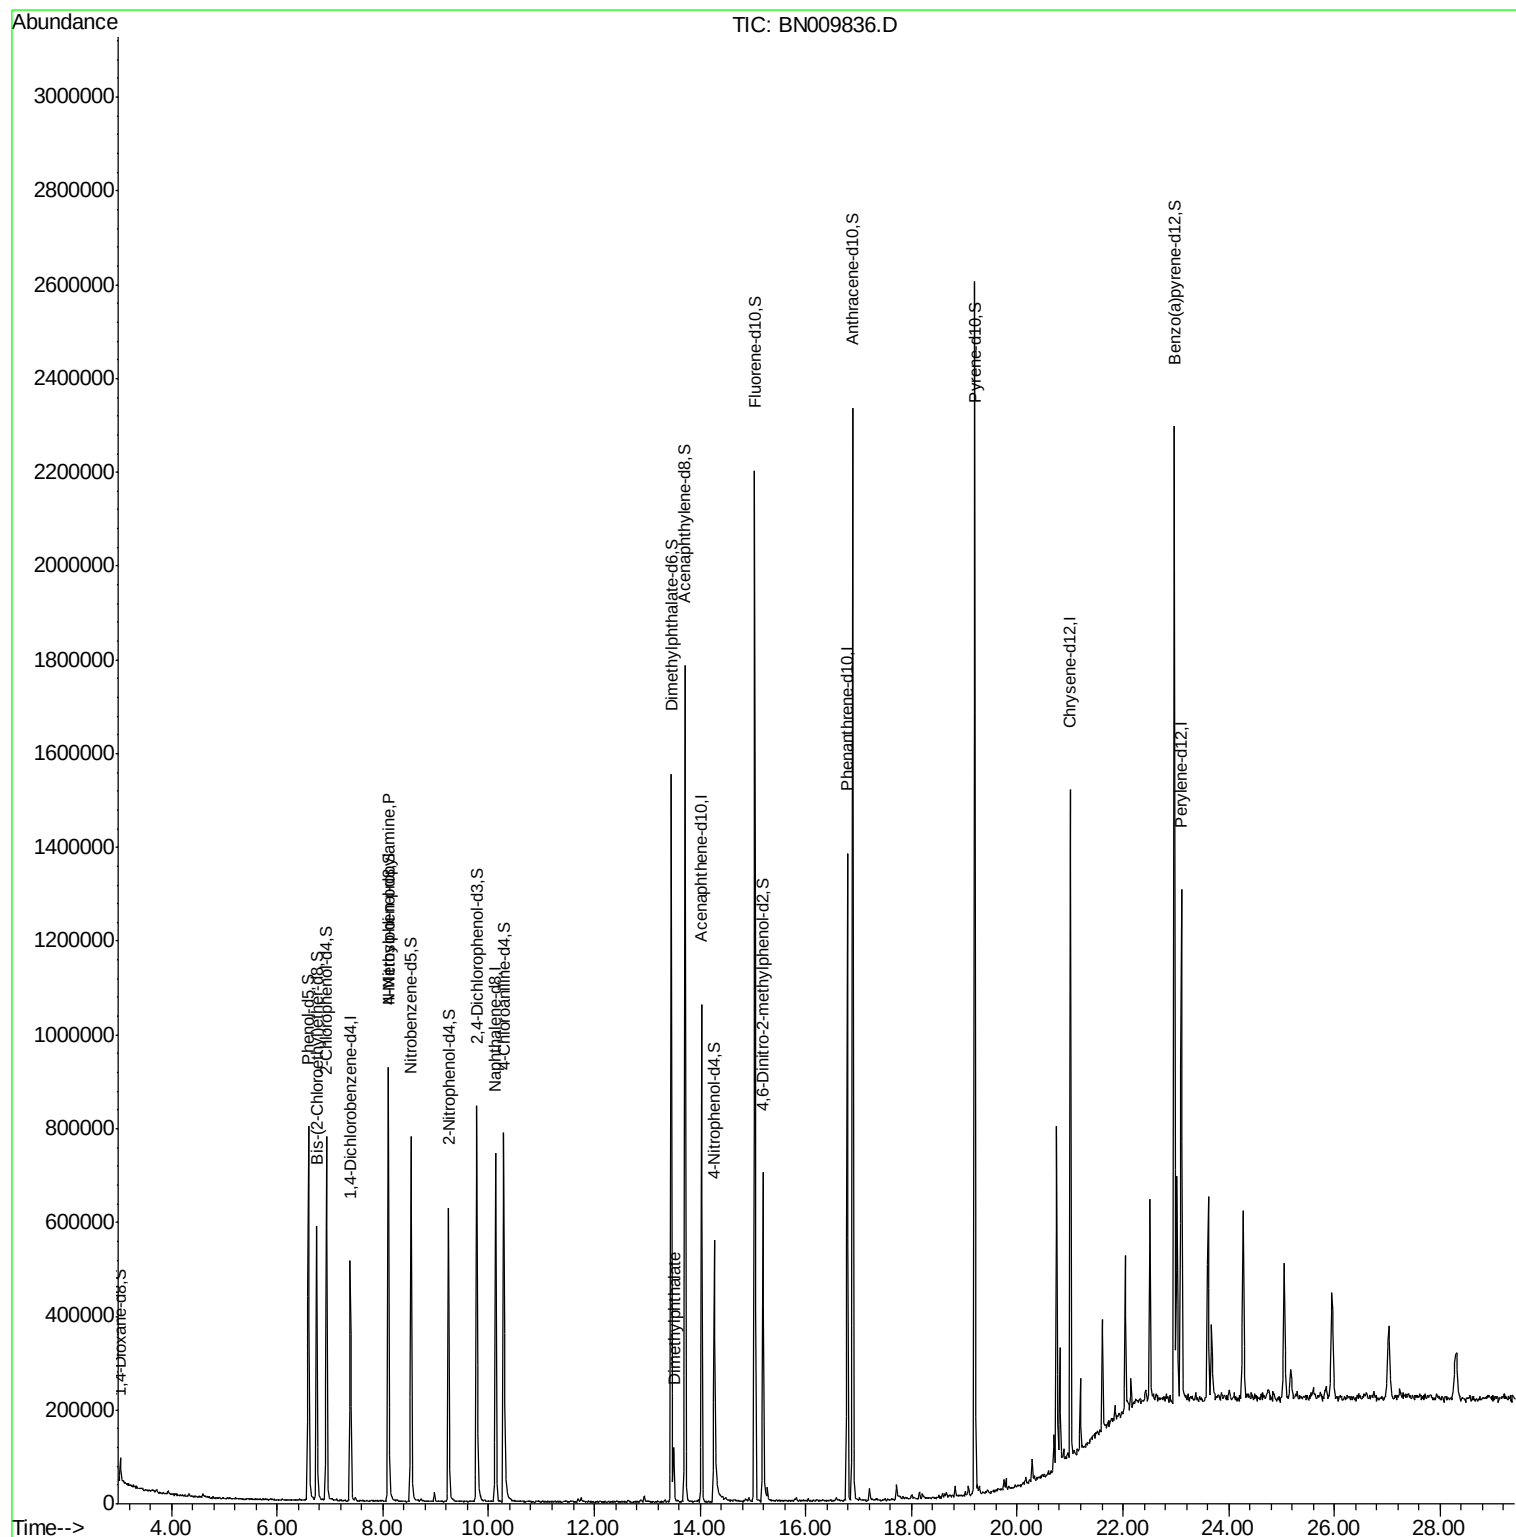

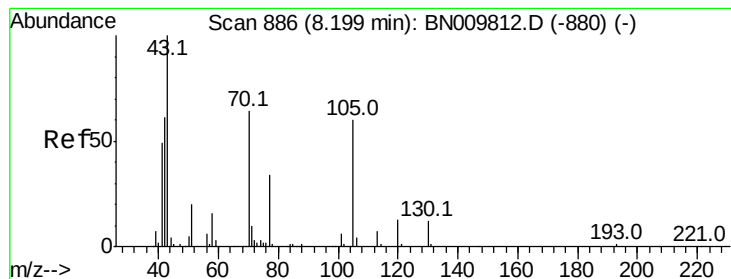

#15

N-Nitroso-di-n-propylamine

Concen: 1.263 ng/ul

RT: 8.10 min Scan# 870

Delta R.T. -0.12 min

Lab File: BN009836.D

Acq: 22 Feb 2020 08:49

Instrument :

BNA_N

ClientSampleId :

Tot Ion: 70 Resp: 8975





Ion Ratio Lower Upper

70 100

42 448.0 72.6 108.8#

101 0.0 7.7 11.5#

130 0.0 14.7 22.1#

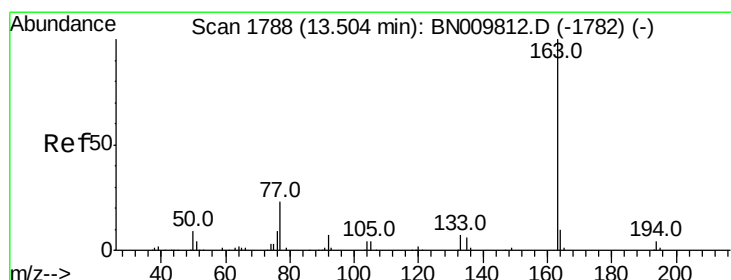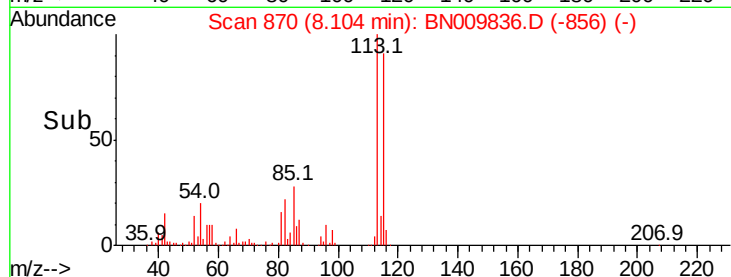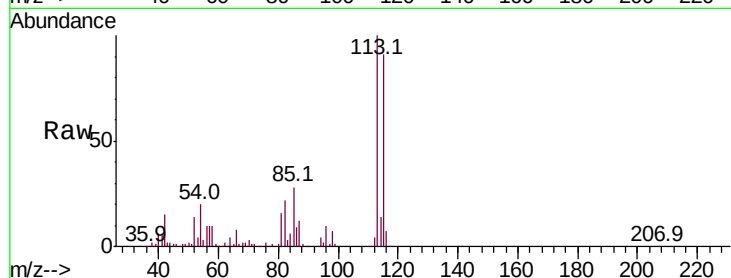

#45

Dimethylphthalate

Concen: 2.377 ng/ul

RT: 13.50 min Scan# 1788

Delta R.T. -0.02 min

Lab File: BN009836.D

Acq: 22 Feb 2020 08:49

Tgt Ion: 163 Resp: 61454

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 9.9 8.0 12.0

