
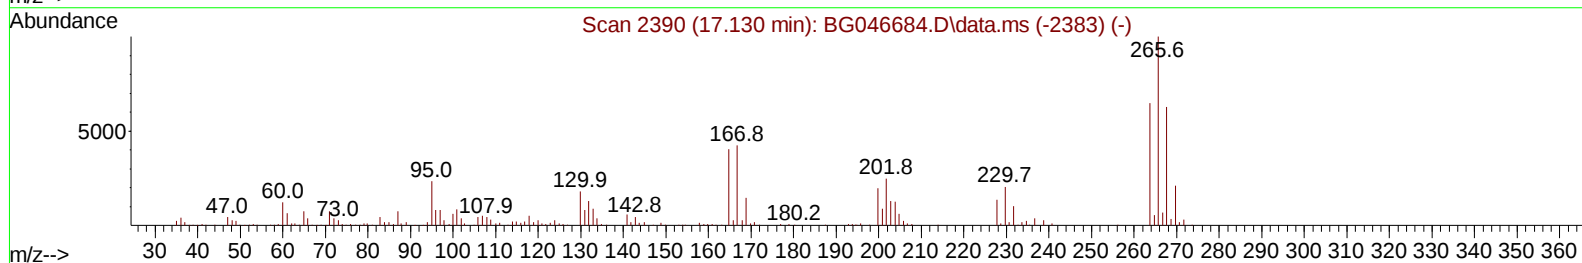
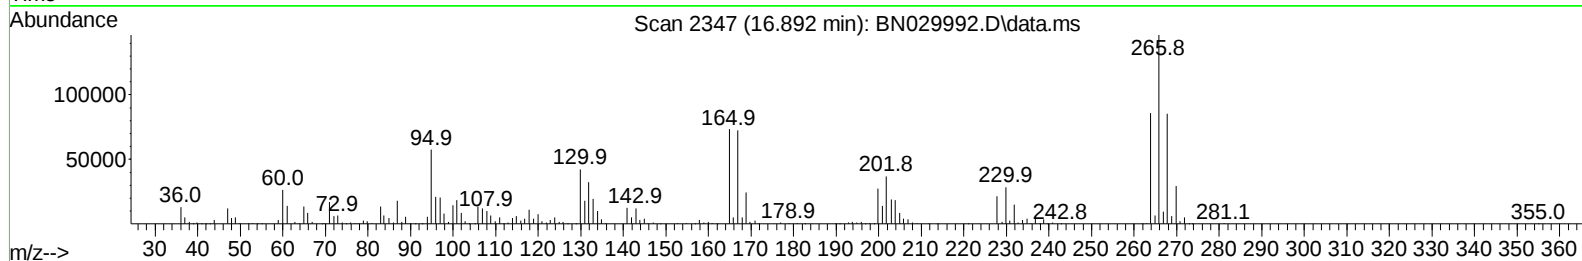


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN029992.D
Acq On : 24 Feb 2024 14:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Feb 26 05:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

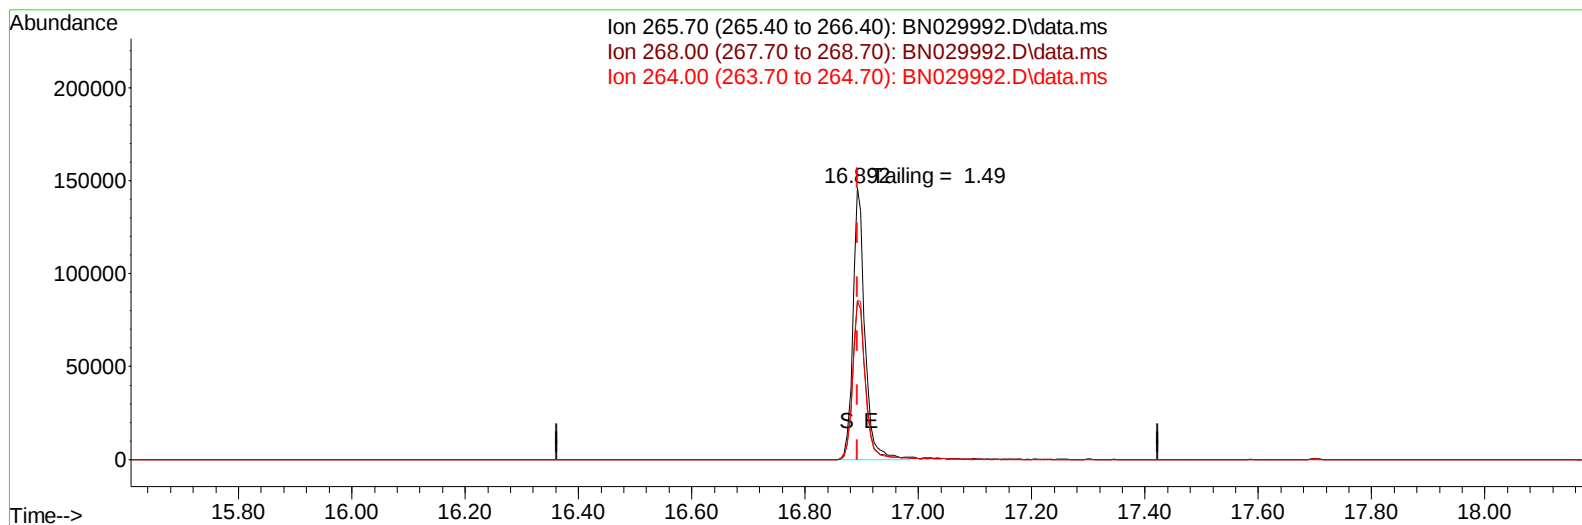

TIC: BN029992.D\data.ms

(70) Pentachlorophenol (C)




16.892min (0.000) 18516.06 ng

response 214186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.26
264.00	61.60	58.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN029992.D
Acq On : 24 Feb 2024 14:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Feb 26 05:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

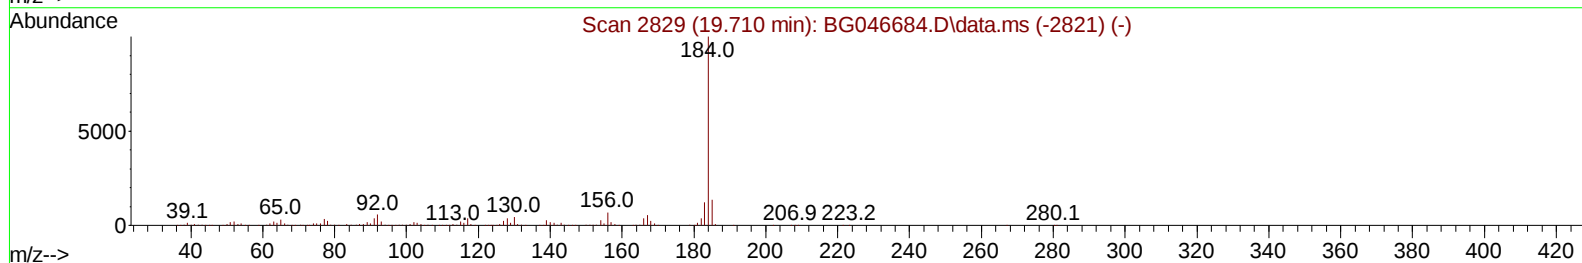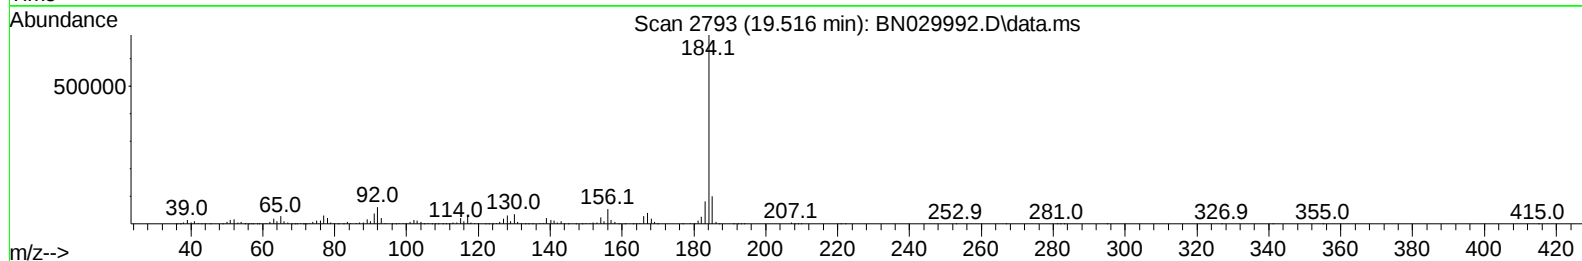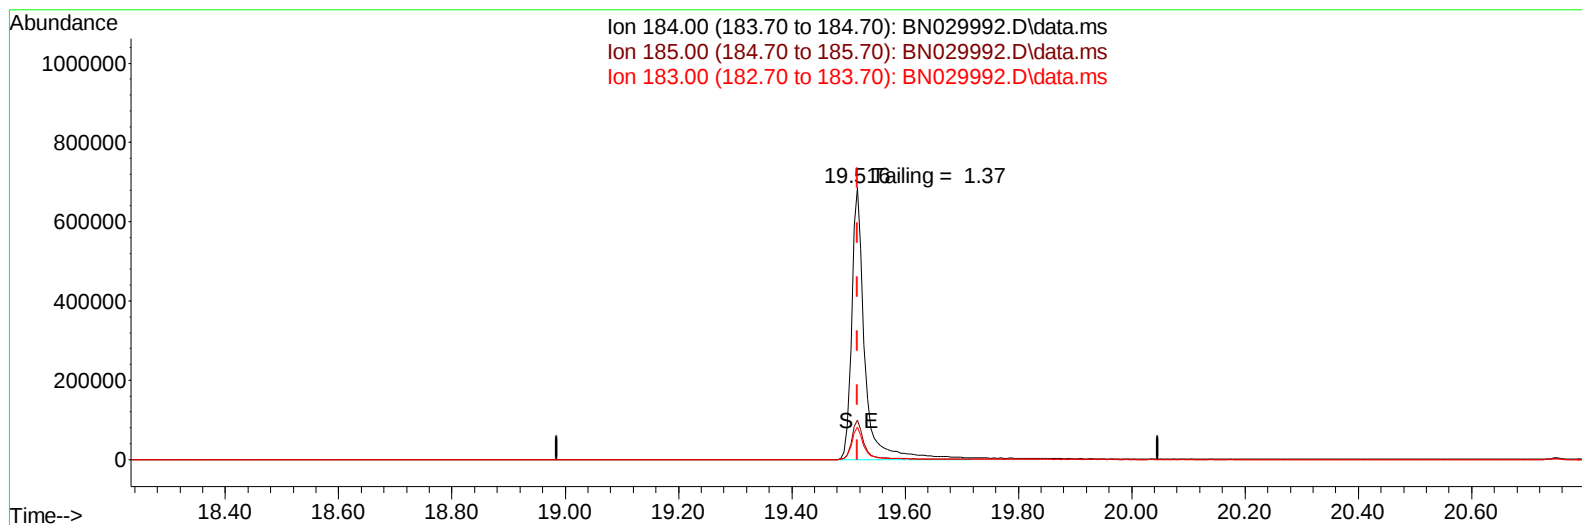

TIC: BN029992.D\data.ms

(77) Benzidine

19.516min (0.000) 0.00 ng

response 1116257

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	11.97
0.00	0.00	0.00