
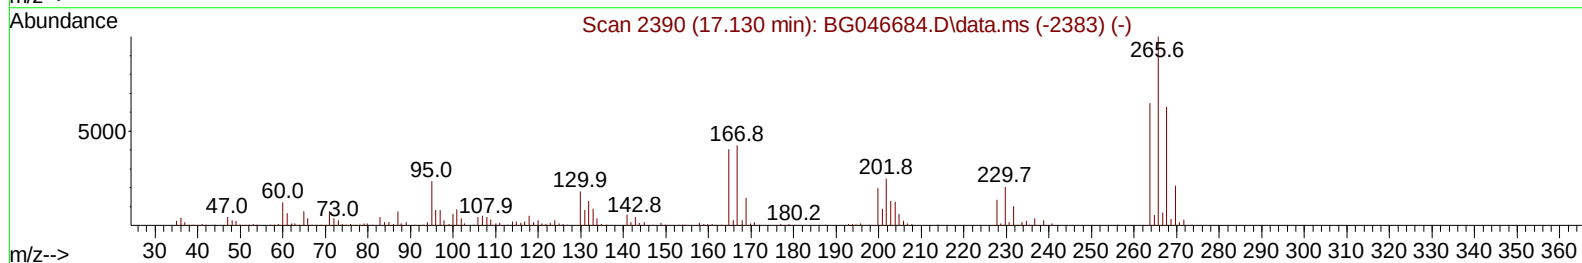
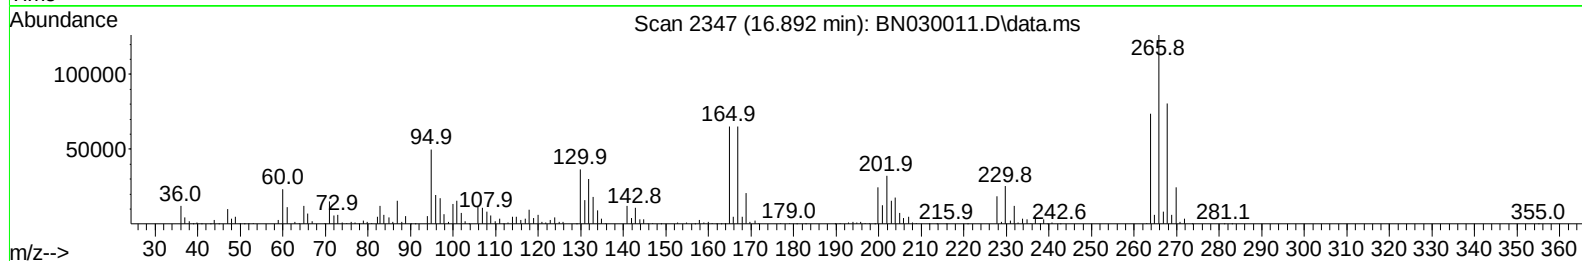


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030011.D
Acq On : 25 Feb 2024 03:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Quant Time: Feb 26 05:02:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

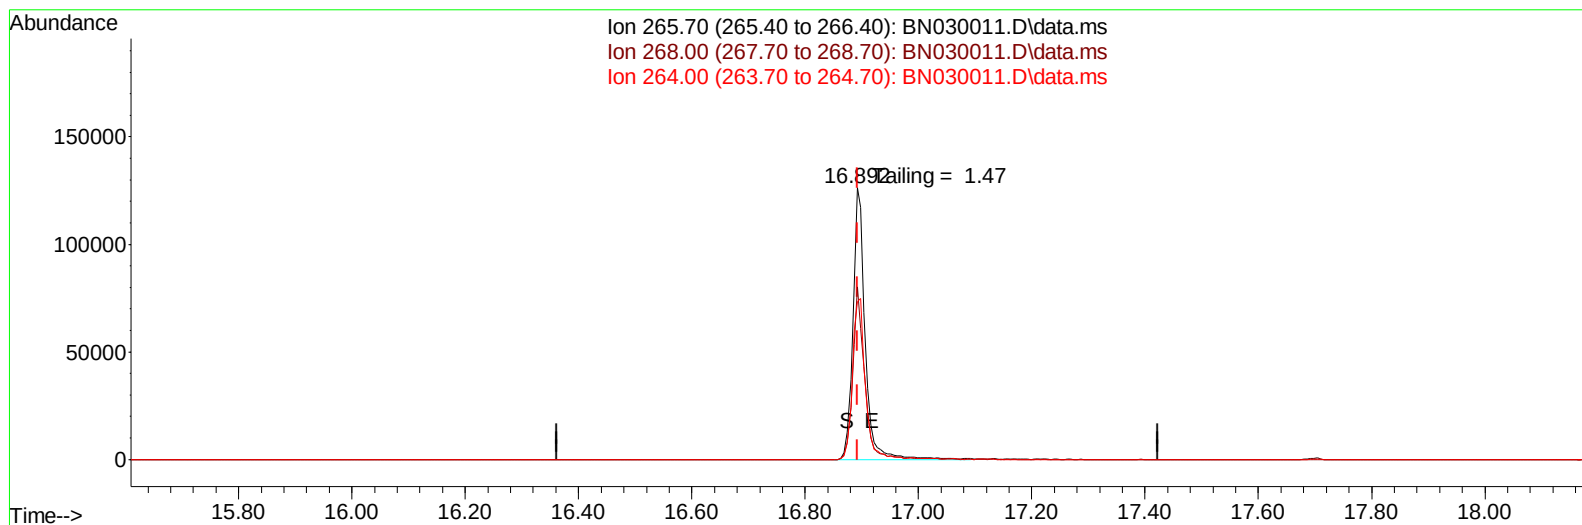

TIC: BN030011.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.000) 16908.32 ng

response 190546

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.63
264.00	61.60	58.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030011.D
Acq On : 25 Feb 2024 03:31
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Quant Time: Feb 26 05:02:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

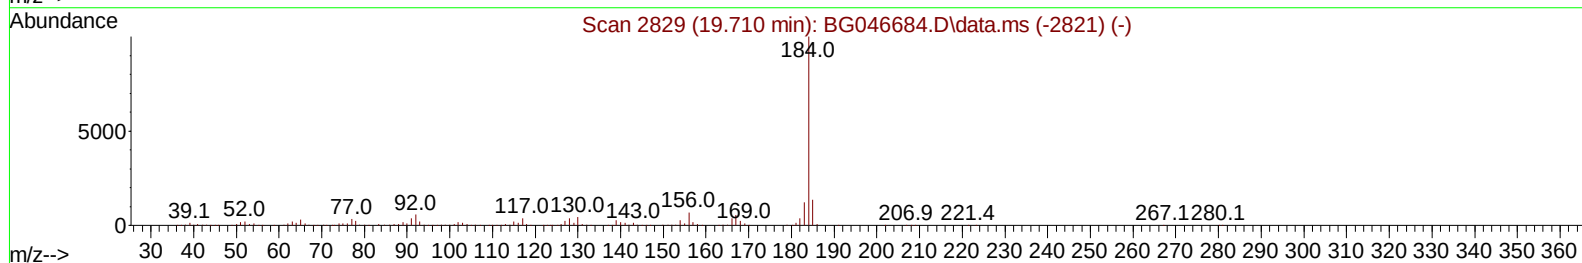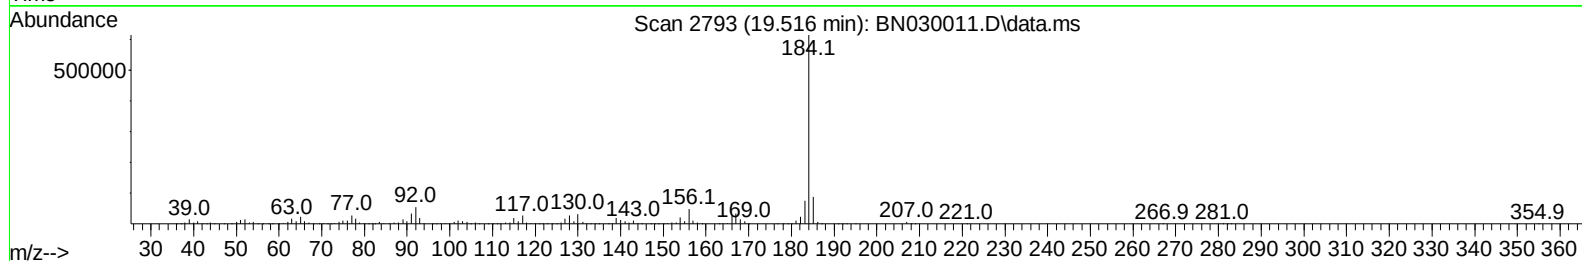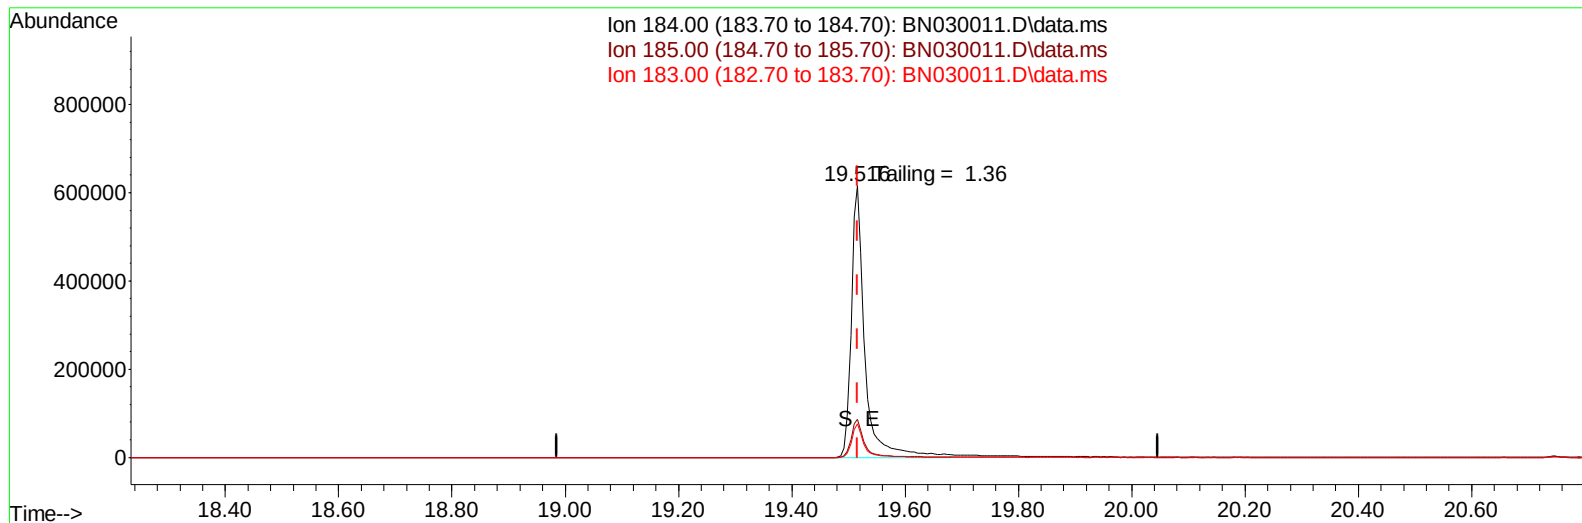

TIC: BN030011.D\data.ms

(77) Benzidine**19.516min (-0.000) 0.00 ng****response 1049275**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.13
183.00	13.20	12.29
0.00	0.00	0.00