
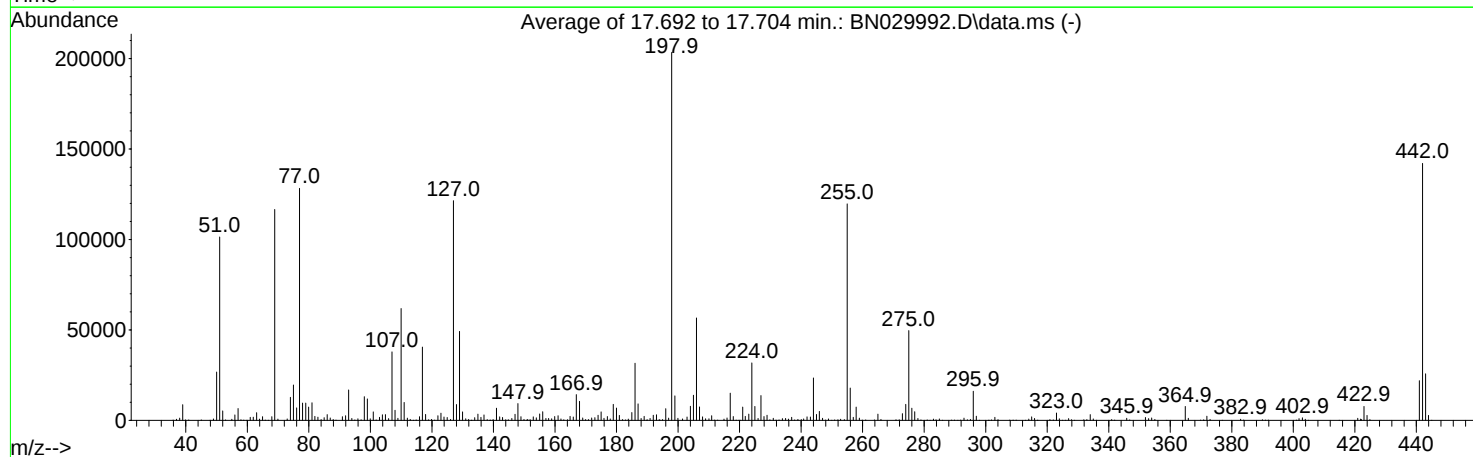


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN029992.D
Acq On : 24 Feb 2024 14:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

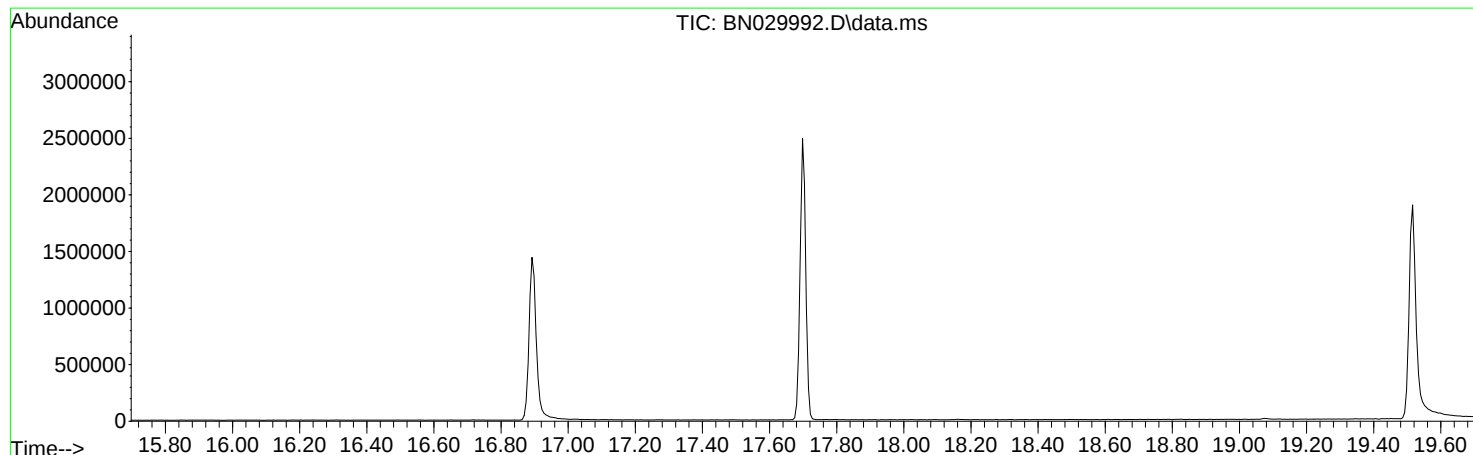




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	101408	PASS
68	69	0.00	2	1.7	2009	PASS
69	198	0.00	100	57.3	116632	PASS
70	69	0.00	2	0.6	741	PASS
127	198	10	80	59.7	121451	PASS
197	198	0.00	2	0.6	1286	PASS
198	198	100	100	100.0	203392	PASS
199	198	5	9	6.6	13510	PASS
275	198	10	60	24.4	49645	PASS
365	198	1	100	3.8	7696	PASS
441	198	0.01	100	10.8	21974	PASS
442	442	50	100	100.0	142080	PASS
443	442	15	24	18.1	25752	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN029992.D
Acq On : 24 Feb 2024 14:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

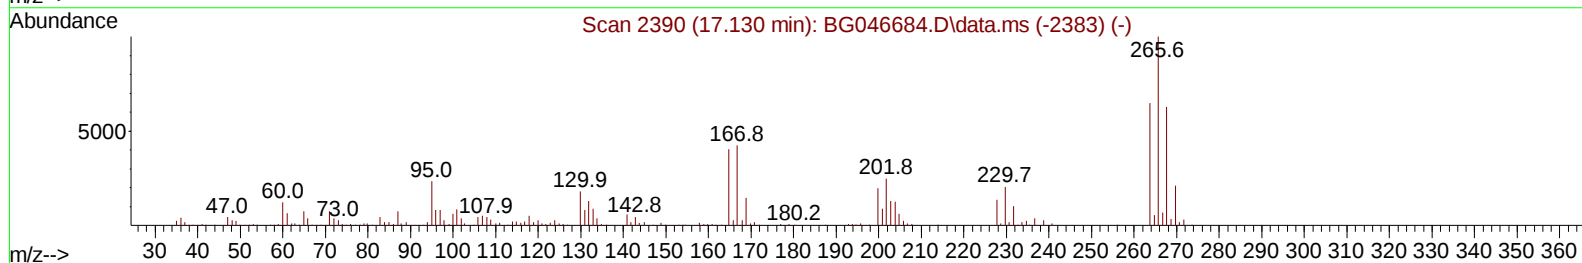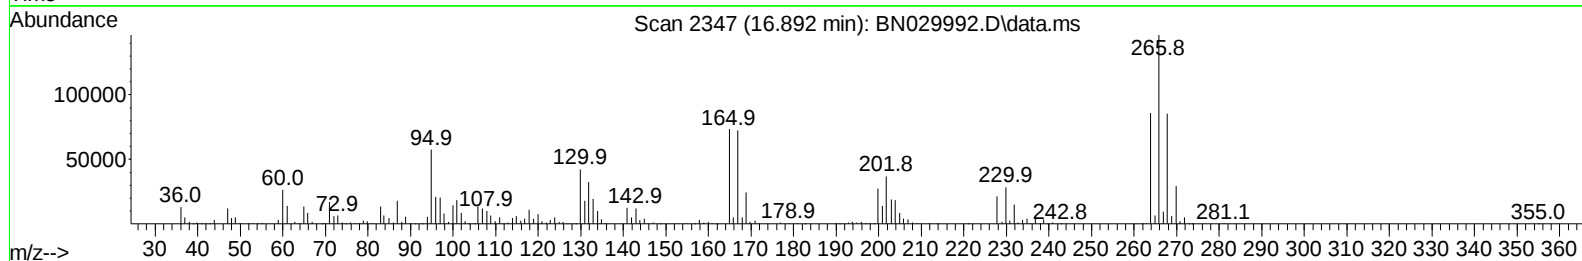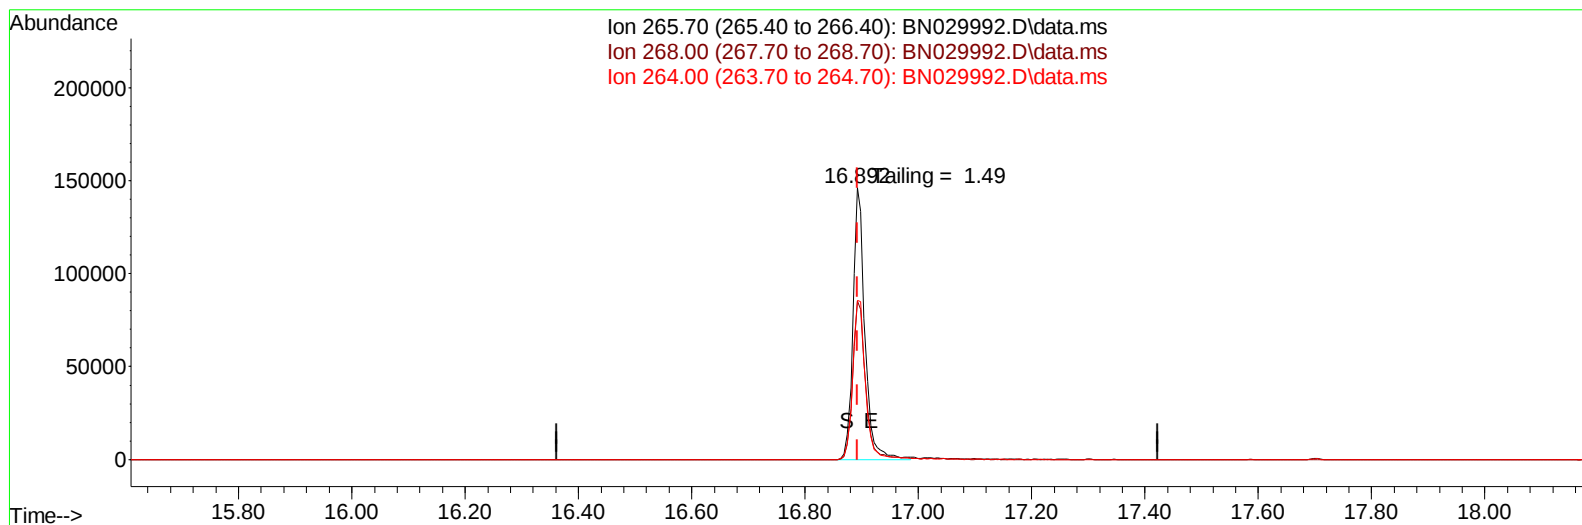

TIC: BN029992.D\data.ms

(70) Pentachlorophenol (C)

16.892min (0.000) 18516.06 ng




response 214186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.26
264.00	61.60	58.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN029992.D
Acq On : 24 Feb 2024 14:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

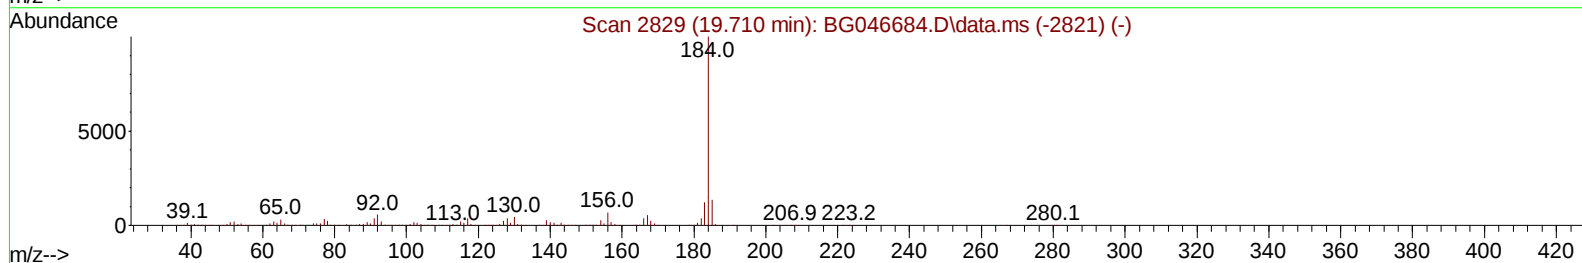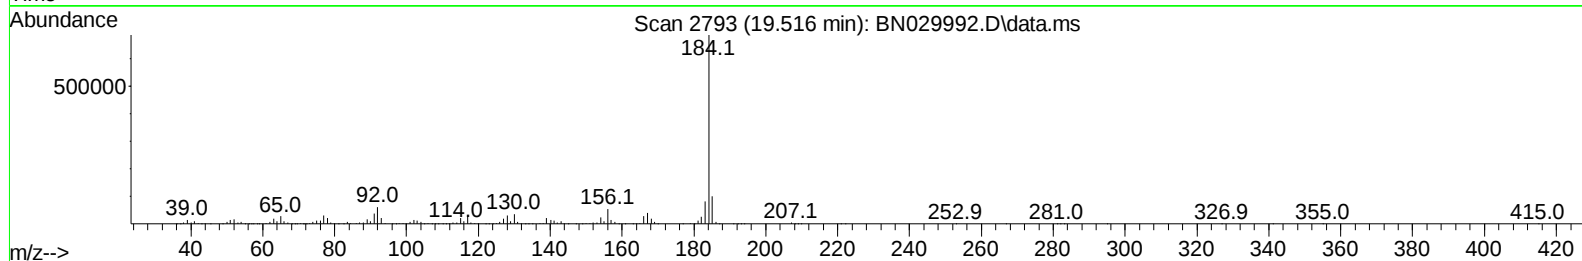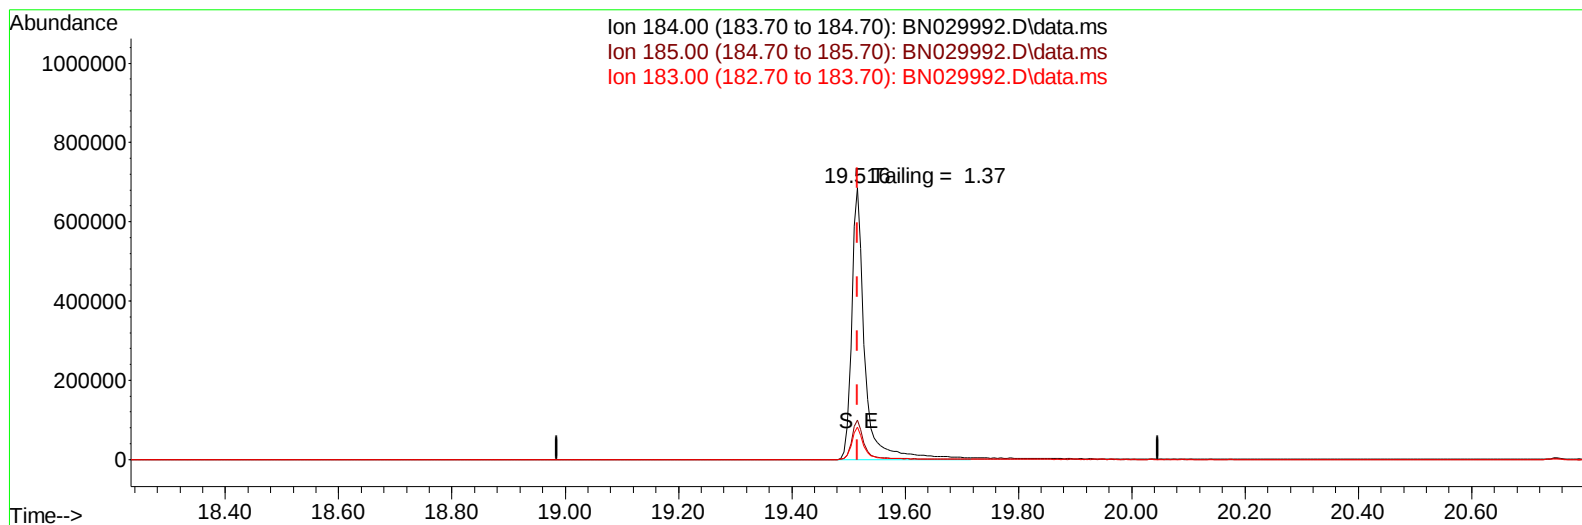

TIC: BN029992.D\data.ms

(77) Benzidine

19.516min (0.000) 0.00 ng

response 1116257

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2024	BNA_N	<u>BN029992.D</u>
Compound Name	Response	Retention Time
DDT	652919	20.751
DDD	13190	20.31
DDE	552	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13742	666661	2.06

Instrument :
BNA_N
ClientSampleId :
DFTPP