
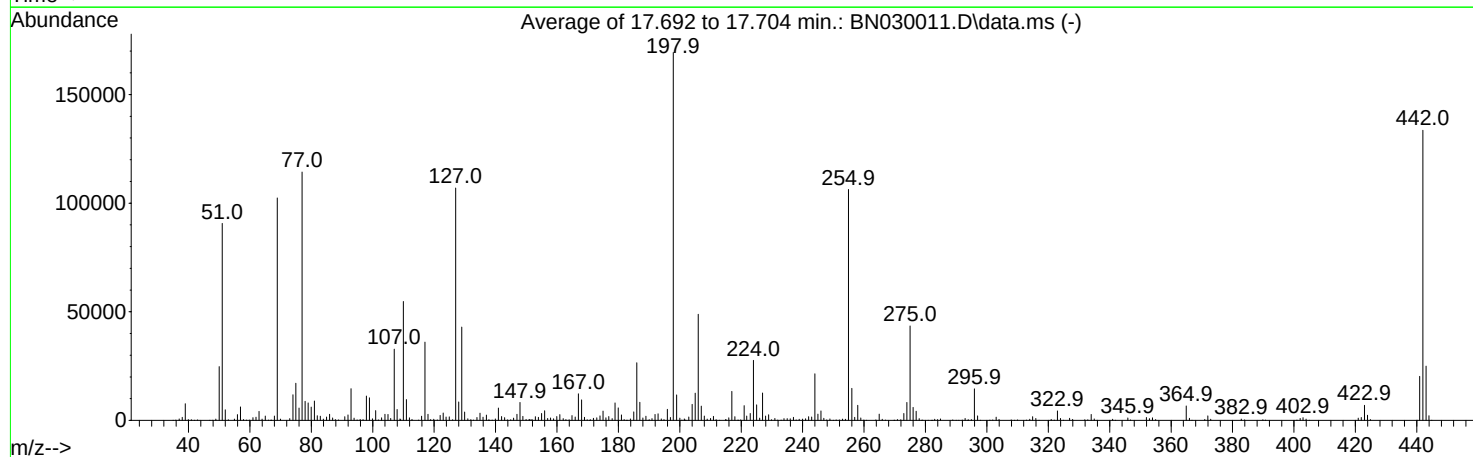


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030011.D
Acq On : 25 Feb 2024 03:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

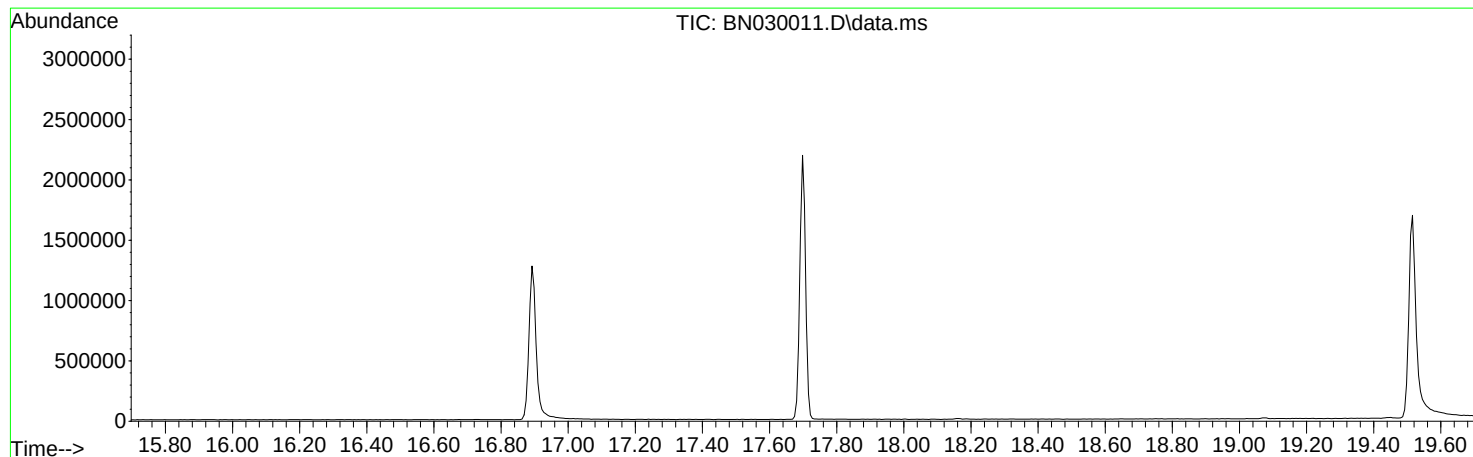




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	90661	PASS
68	69	0.00	2	2.0	2018	PASS
69	198	0.00	100	60.5	102432	PASS
70	69	0.00	2	0.6	569	PASS
127	198	10	80	63.2	106963	PASS
197	198	0.00	2	0.8	1346	PASS
198	198	100	100	100.0	169365	PASS
199	198	5	9	6.9	11735	PASS
275	198	10	60	25.6	43432	PASS
365	198	1	100	3.9	6634	PASS
441	198	0.01	100	11.9	20232	PASS
442	442	50	100	100.0	133549	PASS
443	442	15	24	18.7	24987	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030011.D
Acq On : 25 Feb 2024 03:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:02:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

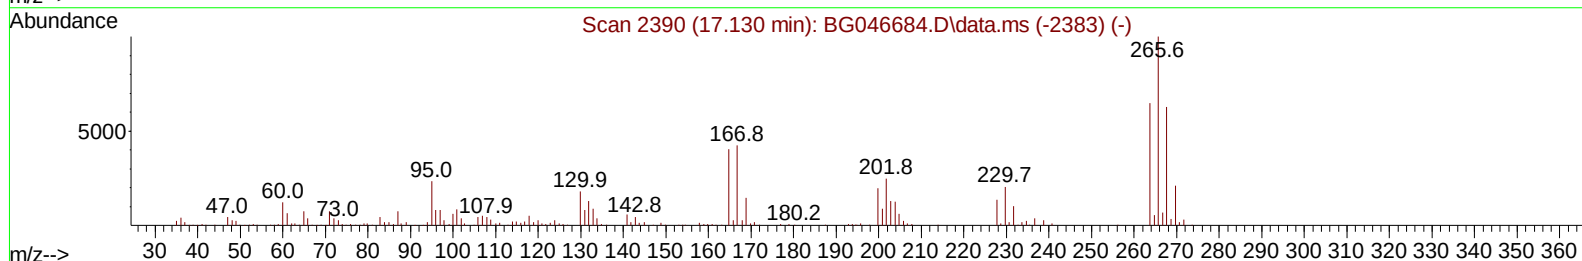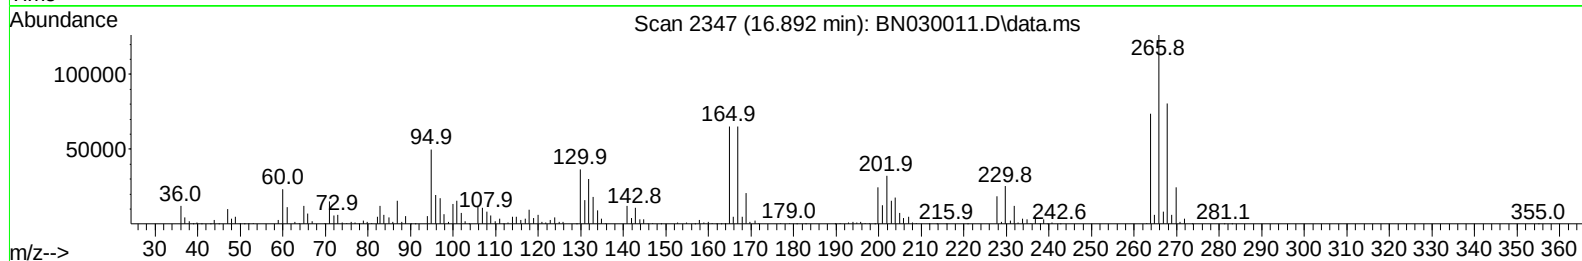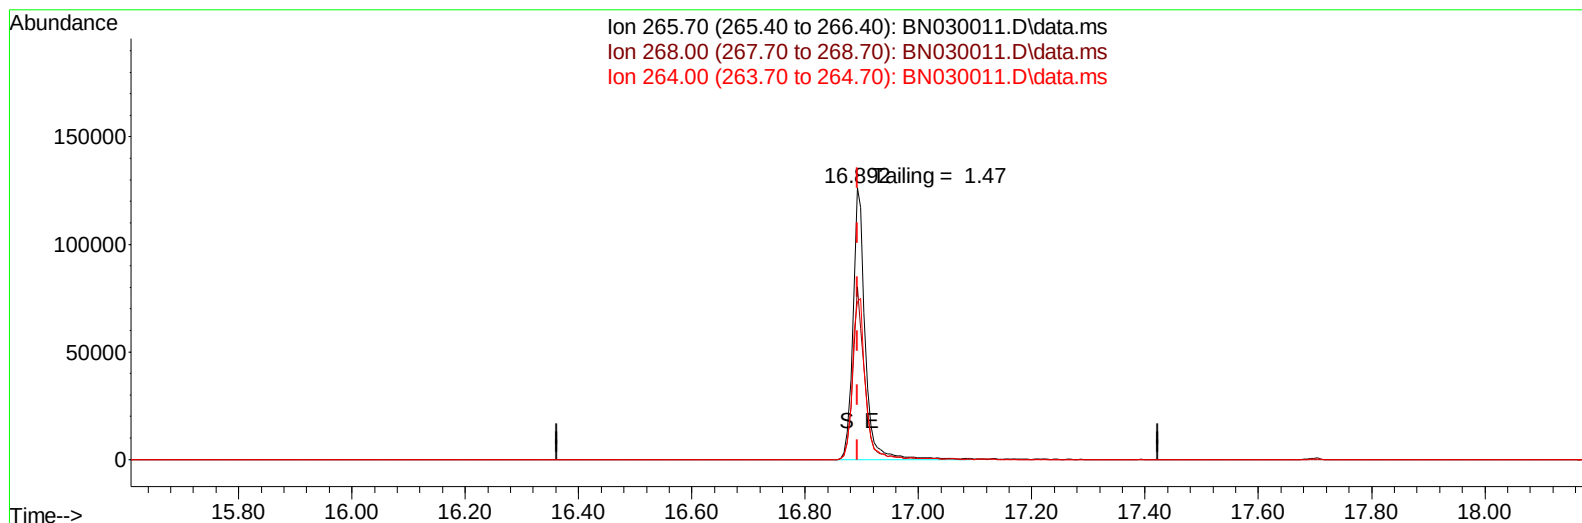

TIC: BN030011.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.000) 16908.32 ng




response 190546

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.63
264.00	61.60	58.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030011.D
Acq On : 25 Feb 2024 03:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:02:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

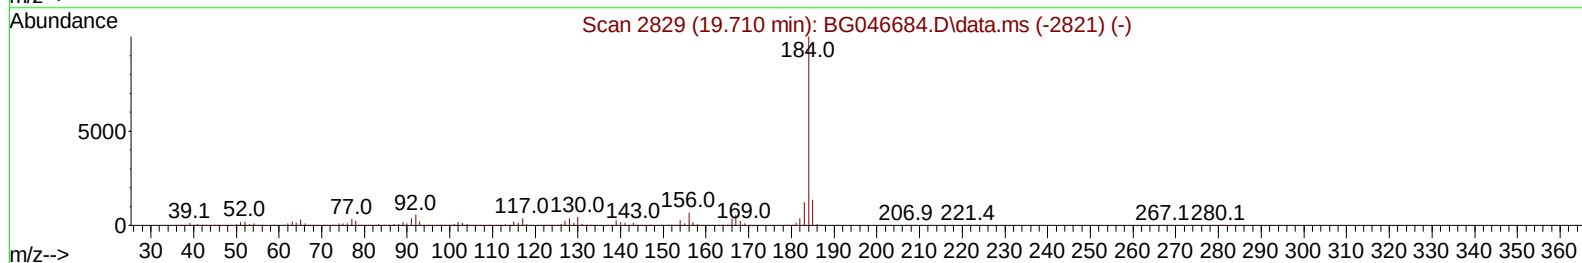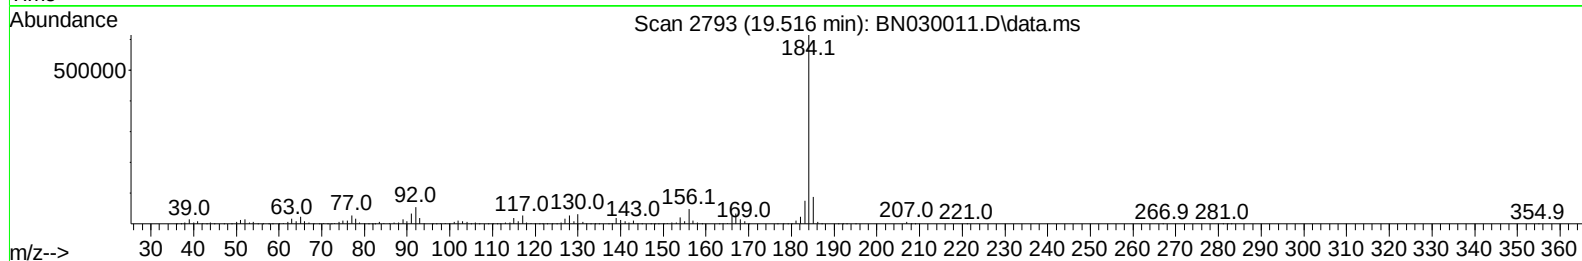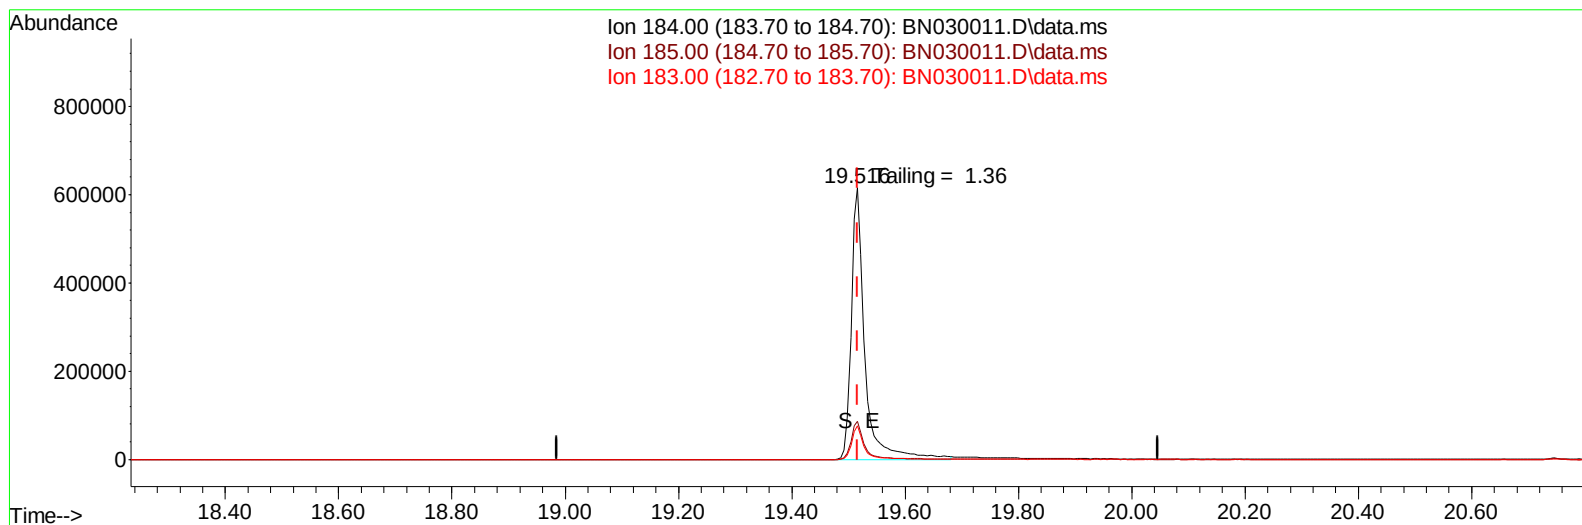

TIC: BN030011.D\data.ms

(77) Benzidine

19.516min (-0.000) 0.00 ng

response 1049275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.13
183.00	13.20	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2024	BNA_N	<u>BN030011.D</u>
Compound Name	Response	Retention Time
DDT	609393	20.745
DDD	14113	20.31
DDE	572	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14685	624078	2.35

Instrument :
BNA_N
ClientSampleId :
DFTPP