
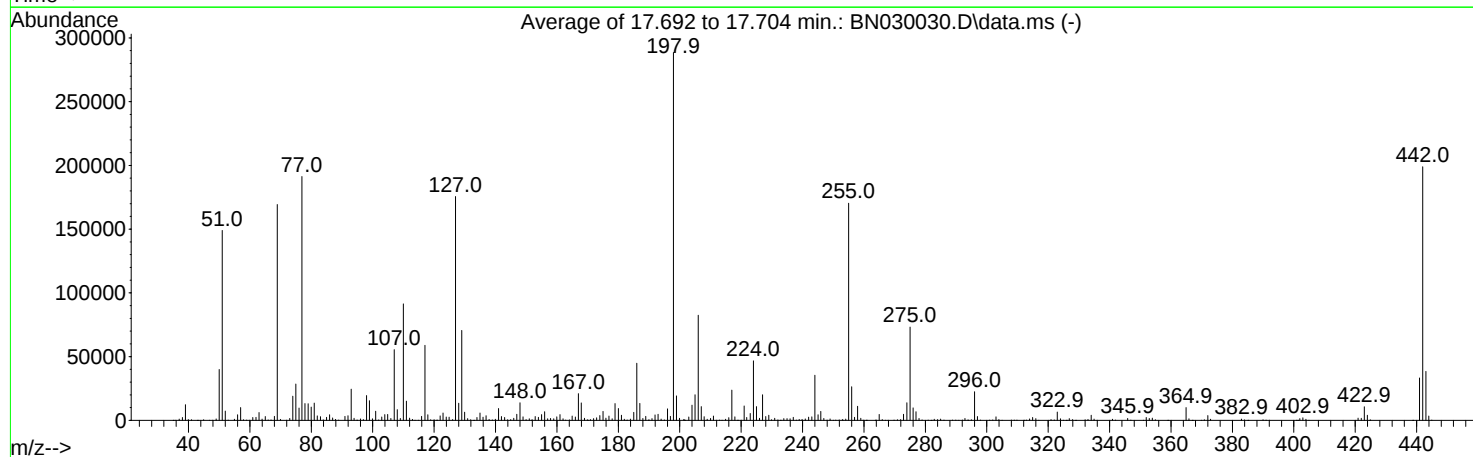


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030030.D
Acq On : 25 Feb 2024 16:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

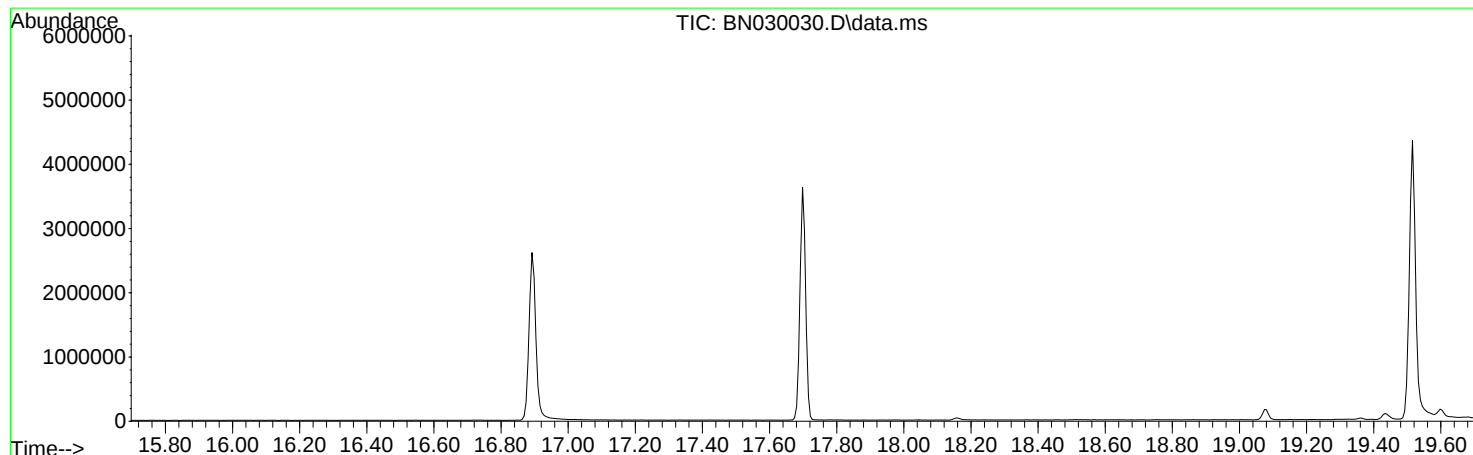




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	51.6	148952	PASS
68	69	0.00	2	1.9	3170	PASS
69	198	0.00	100	58.7	169301	PASS
70	69	0.00	2	0.5	822	PASS
127	198	10	80	60.9	175616	PASS
197	198	0.00	2	1.1	3164	PASS
198	198	100	100	100.0	288555	PASS
199	198	5	9	6.6	19164	PASS
275	198	10	60	25.4	73240	PASS
365	198	1	100	3.5	10020	PASS
441	198	0.01	100	11.5	33285	PASS
442	442	50	100	100.0	198939	PASS
443	442	15	24	19.3	38379	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030030.D
Acq On : 25 Feb 2024 16:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:03:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

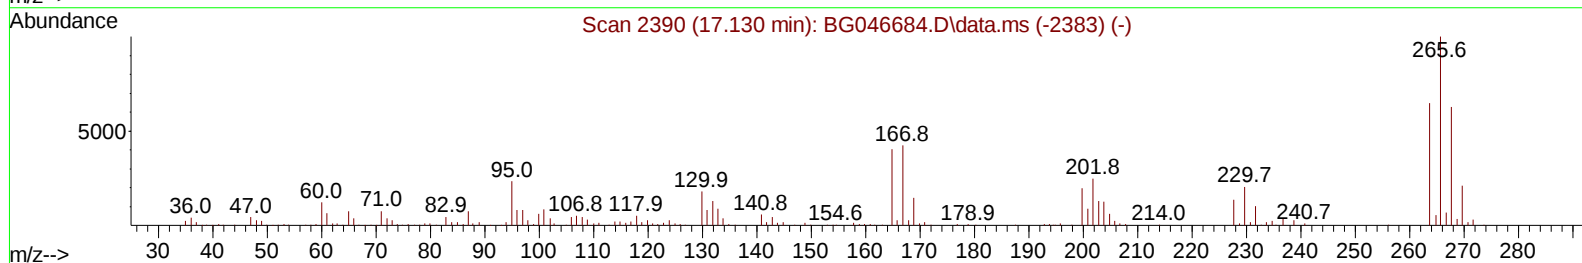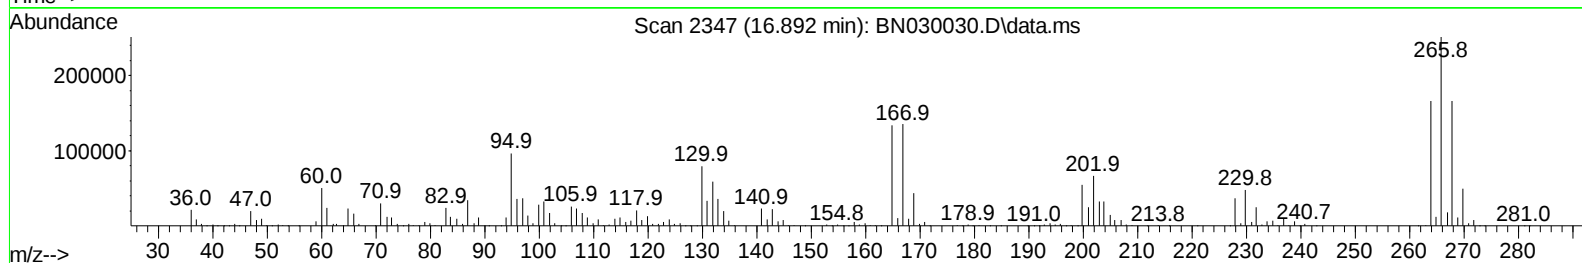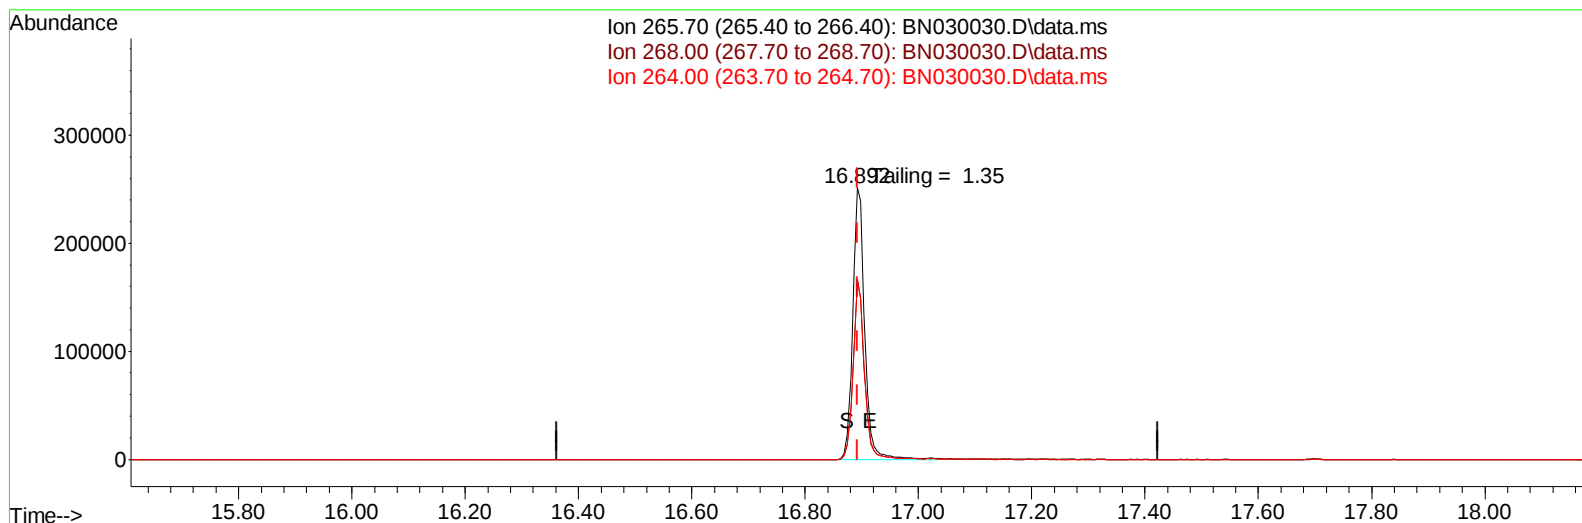

TIC: BN030030.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.000) 21753.47 ng




response 369941

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.22
264.00	61.60	66.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022424\
Data File : BN030030.D
Acq On : 25 Feb 2024 16:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:03:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 05:01:27 2024
Response via : Initial Calibration

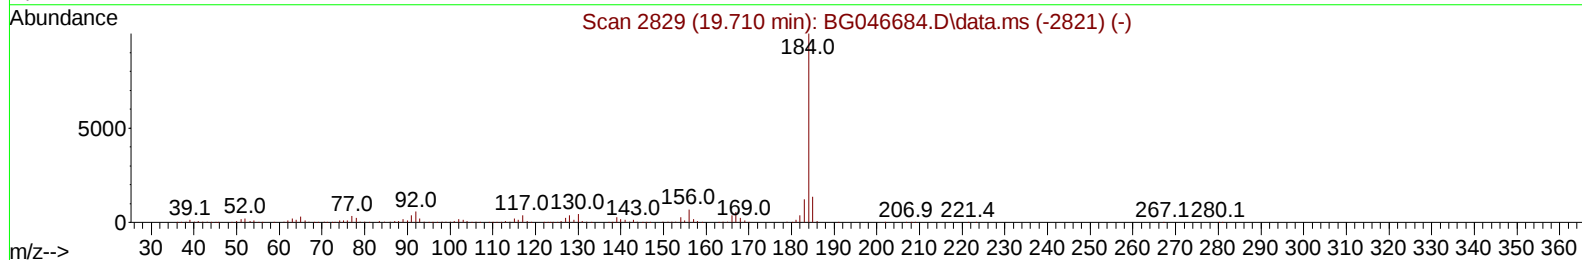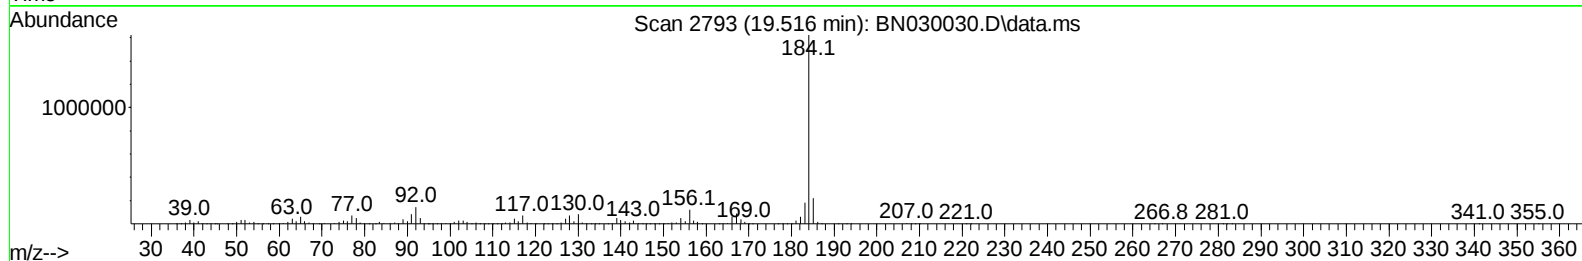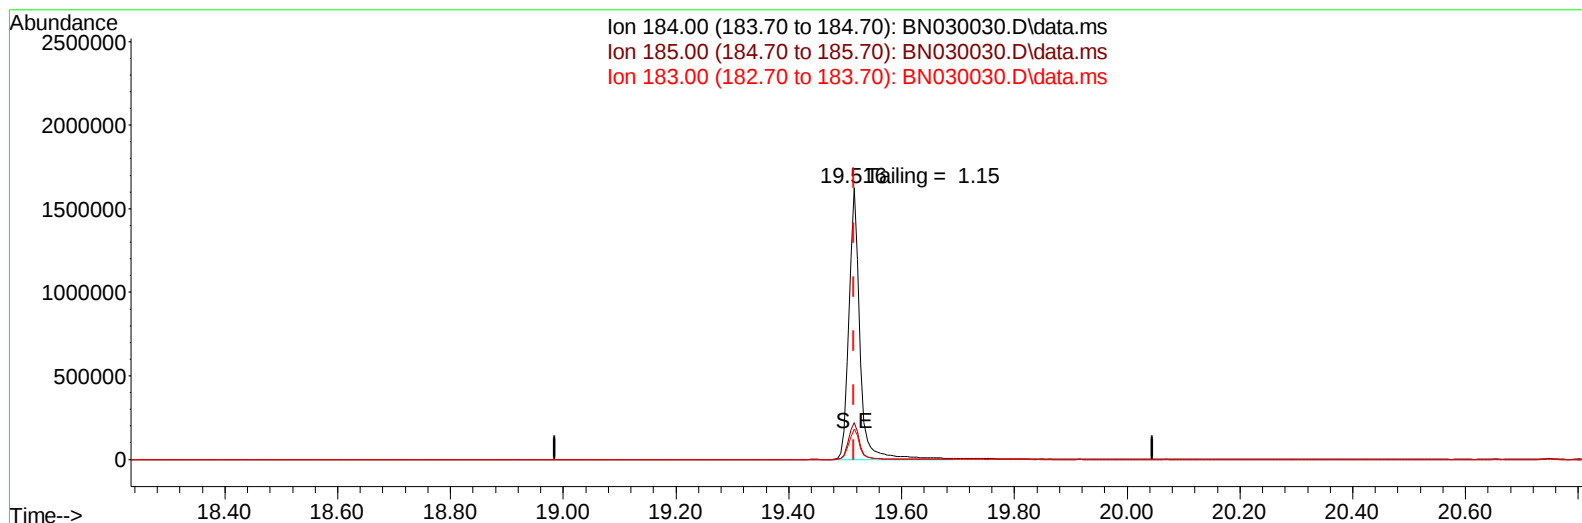

TIC: BN030030.D\data.ms

(77) Benzidine

19.516min (-0.000) 1251682.75 ng

response 2237848

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2024	BNA_N	<u>BN030030.D</u>
Compound Name	Response	Retention Time
DDT	1123069	20.751
DDD	36203	20.31
DDE	1389	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37592	1160661	3.24

Instrument :
BNA_N
ClientSampleId :
DFTPP