

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
 Data File : BN004513.D
 Acq On : 26 Feb 2019 23:41
 Operator : JU/SJ
 Sample : K1552-07RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5Y4RE

Quant Time: Feb 27 05:45:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 27 05:37:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	3372	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	17963	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.37	164	12113	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.12	188	29714	20.00	ng/ul	-0.01
78) Chrysene-d12	21.32	240	44154	20.00	ng/ul	-0.01
86) Perylene-d12	23.58	264	58415	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.24	96	1764	31.45	ng/uL	0.00
5) Phenol-d5	6.89	99	17744	59.05	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.08	67	33366	221.27	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.26	132	51560	211.56	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	34158	132.24	ng/ul	-0.01
19) Nitrobenzene-d5	8.90	128	29567	248.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.61	143	33907	273.16	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.14	165	63832	226.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	3534	11.35	ng/ul	-0.01
44) Dimethylphthalate-d6	13.79	166	231112	224.98	ng/ul	-0.01
47) Acenaphthylene-d8	14.07	160	288907	237.41	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.57	143	8865	45.08	ng/ul	-0.01
58) Fluorene-d10	15.37	176	218430	241.54	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.49	200	35164	202.93	ng/ul	-0.01
71) Anthracene-d10	17.22	188	360882	253.42	ng/ul	-0.01
79) Pyrene-d10	19.52	212	475015	240.03	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.45	264	779501	254.26	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
84) Bis(2-ethylhexyl)phthalate	21.22	149	5926	4.712	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004513.D
Acq On : 26 Feb 2019 23:41
Operator : JU/SJ
Sample : K1552-07RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5Y4RE

Quant Time: Feb 27 05:45:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 27 05:37:09 2019
Response via : Initial Calibration

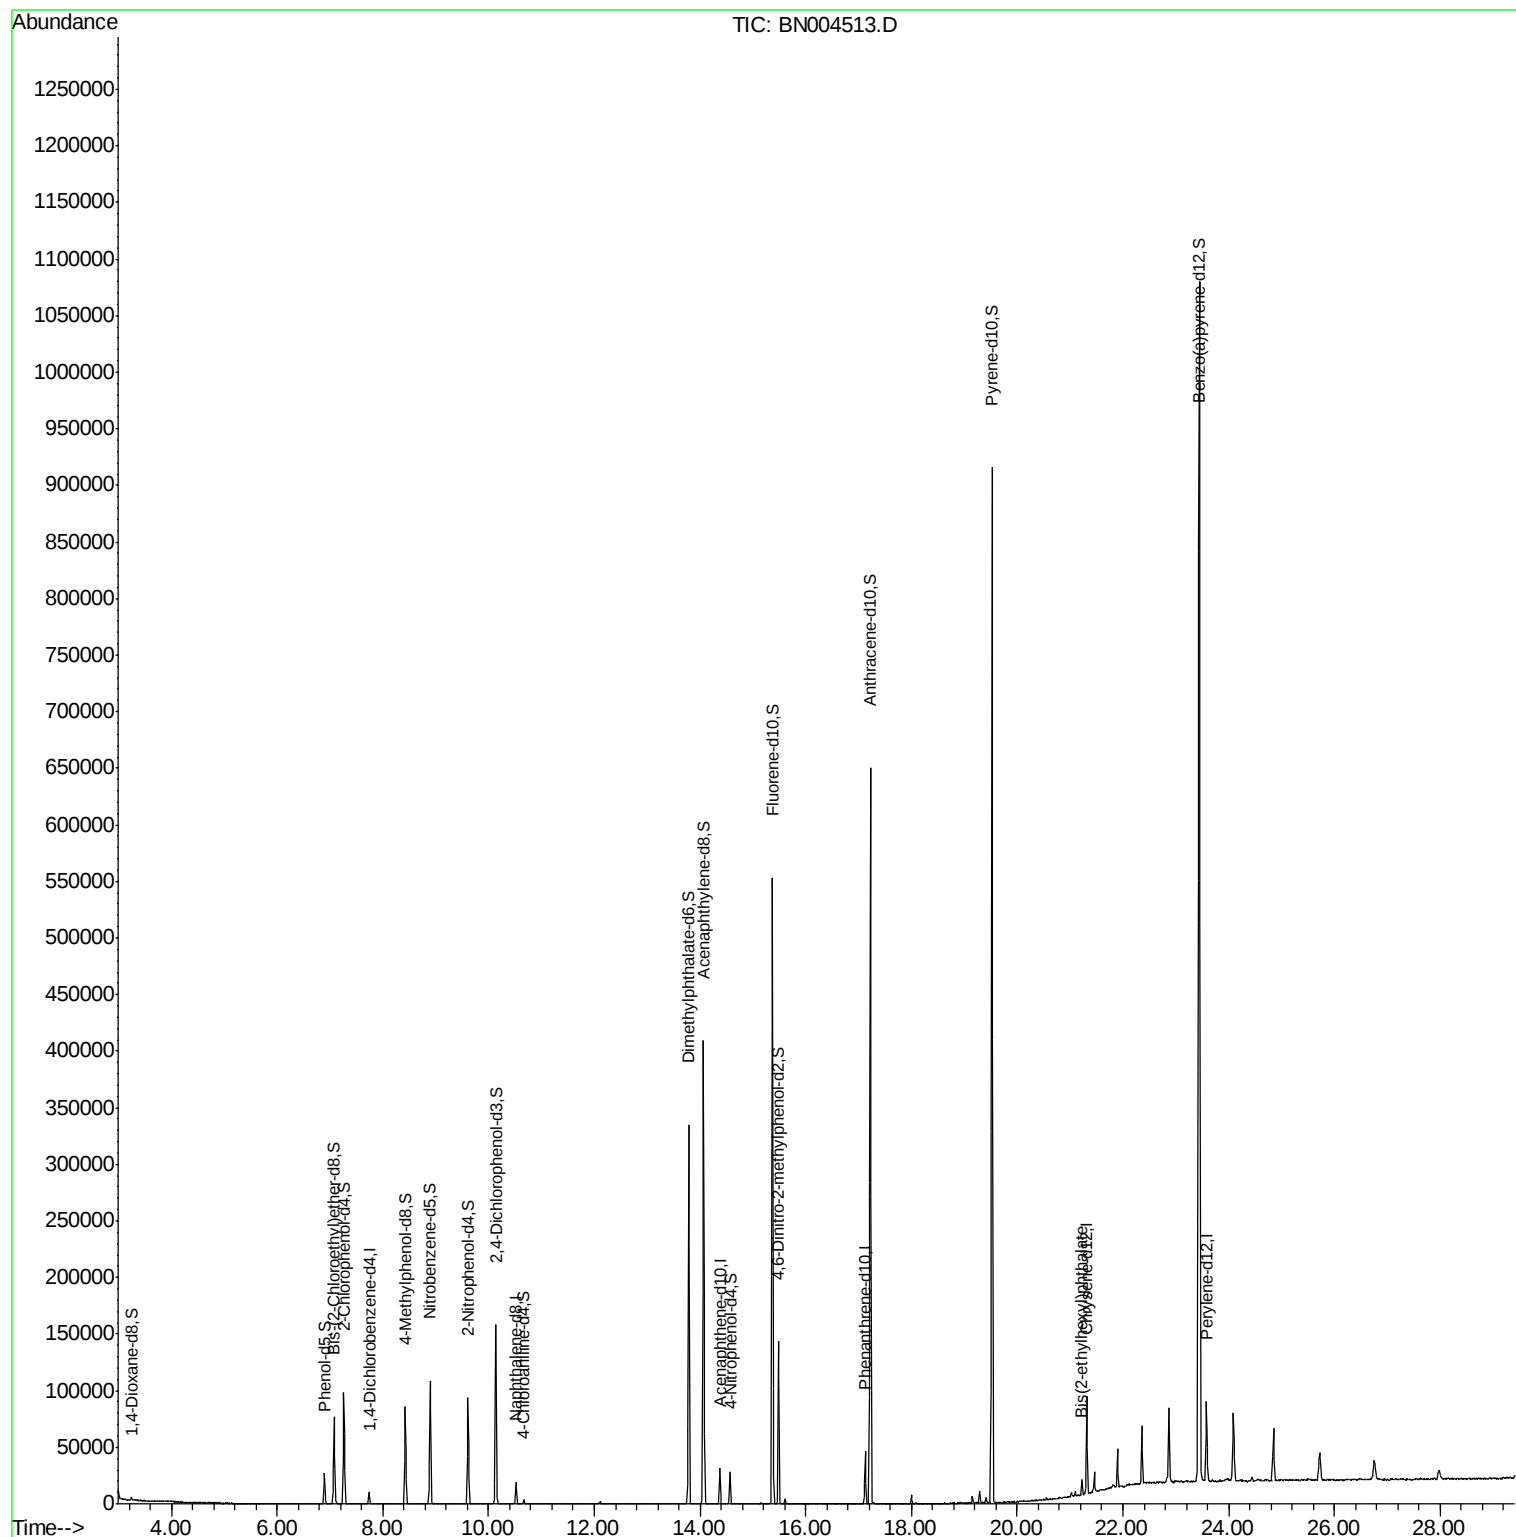

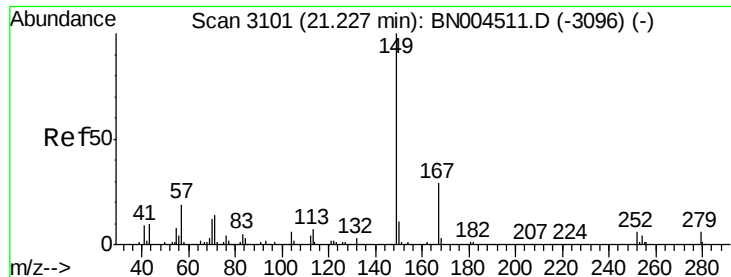

#84

Bis(2-ethylhexyl)phthalate

Concen: 4.712 ng/ul

RT: 21.22 min Scan# 3100

Delta R.T. -0.02 min

Lab File: BN004513.D

Acq: 26 Feb 2019 23:41

Instrument :

BNA_N

ClientSampleId :

BF5Y4RE


Tot Ion:149 Resp: 5926

Ion Ratio Lower Upper

149 100

167 27.8 22.7 34.1

279 0.0 4.3 6.5#

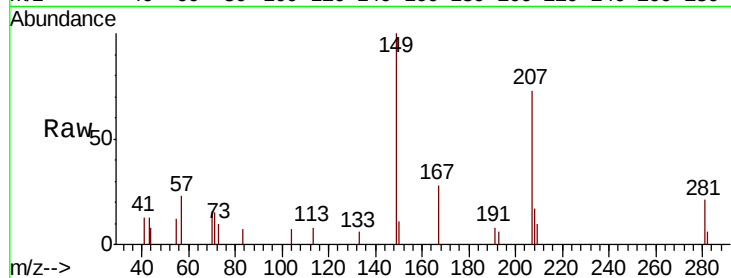

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

