

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
 Data File : BN004514.D
 Acq On : 27 Feb 2019 00:16
 Operator : JU/SJ
 Sample : K1553-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5W9

Quant Time: Feb 27 05:41:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 27 05:37:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	33117	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	161563	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.37	164	103063	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.12	188	253634	20.00	ng/ul	-0.01
78) Chrysene-d12	21.32	240	368178	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	432837	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.24	96	2872	5.21	ng/uL	0.00
5) Phenol-d5	6.89	99	35624	12.07	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.08	67	18143	12.25	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.26	132	32144	13.43	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	30299	11.94	ng/ul	-0.01
19) Nitrobenzene-d5	8.90	128	15136	14.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.61	143	16467	14.75	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.13	165	35755	14.13	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	31828	11.37	ng/ul	-0.01
44) Dimethylphthalate-d6	13.79	166	115324	13.19	ng/ul	-0.01
47) Acenaphthylene-d8	14.07	160	135478	13.08	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.57	143	15320	9.16	ng/ul	-0.01
58) Fluorene-d10	15.37	176	107057	13.91	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.49	200	12527	8.47	ng/ul	-0.01
71) Anthracene-d10	17.22	188	166094	13.66	ng/ul	-0.01
79) Pyrene-d10	19.52	212	207840	12.59	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.44	264	293904	12.94	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.83	163	19371	2.242	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022619\
Data File : BN004514.D
Acq On : 27 Feb 2019 00:16
Operator : JU/SJ
Sample : K1553-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5W9

Quant Time: Feb 27 05:41:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 27 05:37:09 2019
Response via : Initial Calibration

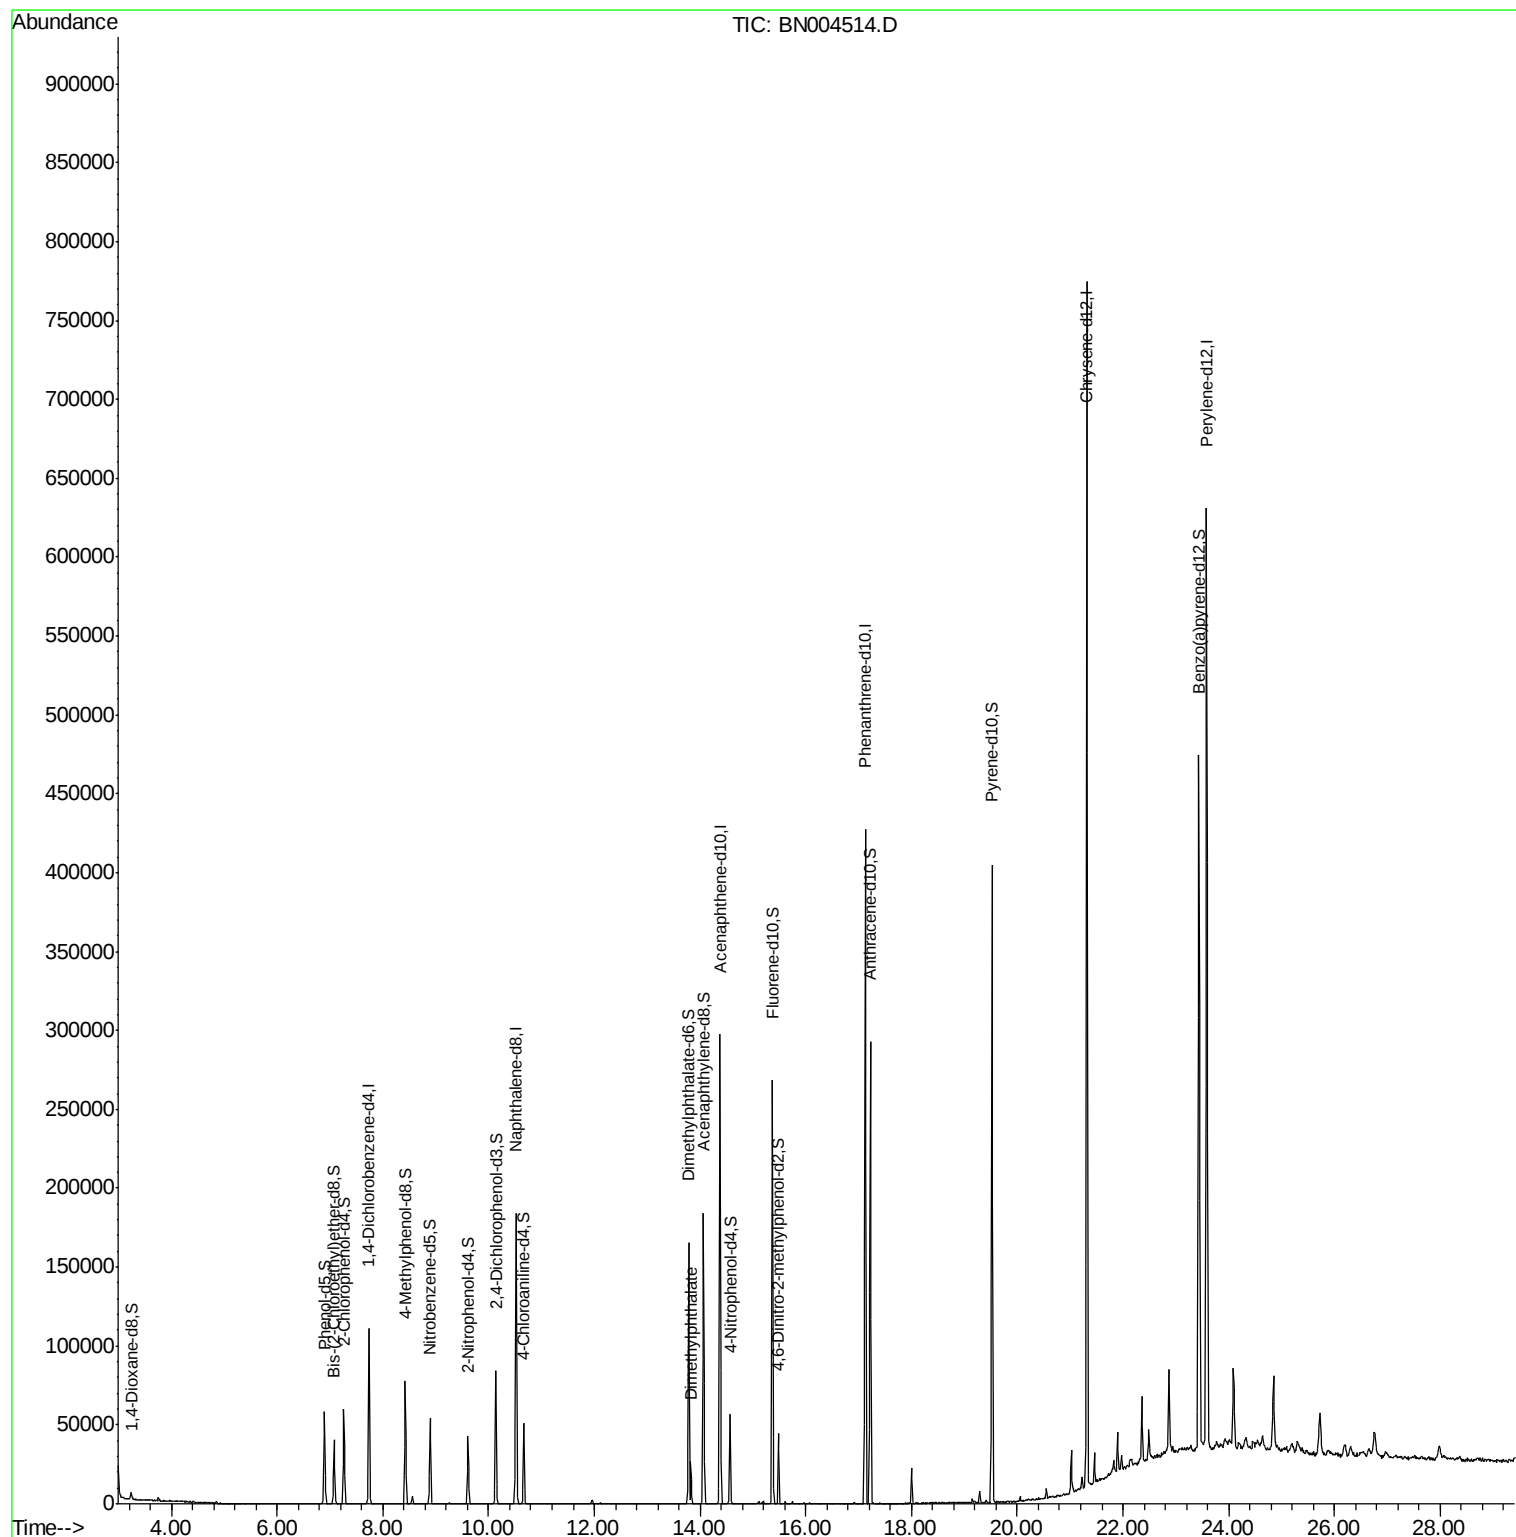

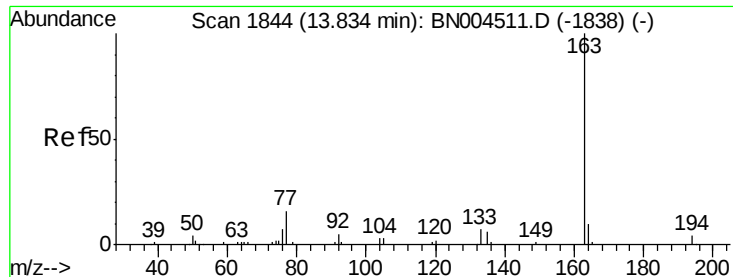

#45

Dimethylphthalate

Concen: 2.242 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004514.D

Acq: 27 Feb 2019 00:16

Instrument :

BNA_N

ClientSampleId :

BF5W9


Tot Ion:163 Resp: 19371

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.2

164 11.7 7.9 11.9

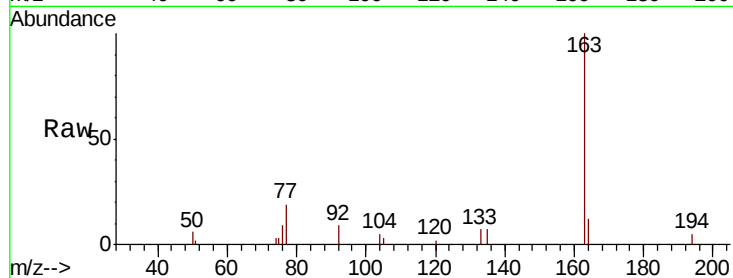

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

