

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022619\
 Data File : BN004504.D
 Acq On : 26 Feb 2019 18:22
 Operator : JU/SJ
 Sample : K1553-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5X2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	48	rVB	2631	4251	0.49%	0.073%
2	6.893	659	664	674	rBB2	39595	74794	8.61%	1.278%
3	7.075	690	695	705	rBB	28215	45455	5.24%	0.777%
4	7.264	722	727	734	rBB	42204	62235	7.17%	1.064%
5	7.740	802	808	814	rBB	68923	106799	12.30%	1.826%
6	8.428	920	925	931	rBB	56204	82057	9.45%	1.403%
7	8.564	944	948	951	rBB	1761	2598	0.30%	0.044%
8	8.899	999	1005	1011	rBB	40161	62228	7.17%	1.064%
9	9.611	1121	1126	1132	rBB	30200	43851	5.05%	0.750%
10	10.140	1210	1216	1222	rBB	60697	90881	10.47%	1.553%
11	10.522	1275	1281	1288	rBB	122471	190613	21.95%	3.258%
12	10.663	1299	1305	1313	rBB	54079	84587	9.74%	1.446%
13	13.787	1830	1836	1840	rBV	128179	174547	20.10%	2.984%
14	13.834	1840	1844	1848	rVB	21776	27659	3.19%	0.473%
15	14.069	1878	1884	1893	rBB	142802	201958	23.26%	3.452%
16	14.375	1931	1936	1942	rBB2	206724	300478	34.61%	5.136%
17	14.569	1964	1969	1974	rBB	38570	50826	5.85%	0.869%
18	15.369	2100	2105	2111	rBB	216967	293742	33.83%	5.021%
19	15.487	2121	2125	2130	rBB	32941	38349	4.42%	0.655%
20	17.122	2397	2403	2410	rBB2	294787	404914	46.63%	6.921%
21	17.222	2414	2420	2430	rBB	240074	318918	36.73%	5.451%
22	17.887	2528	2533	2539	rVB	3898	4917	0.57%	0.084%
23	18.004	2550	2553	2559	rBV	20269	22580	2.60%	0.386%
24	19.157	2745	2749	2752	rBV2	1949	2571	0.30%	0.044%
25	19.292	2768	2772	2778	rBV	8850	9364	1.08%	0.160%
26	19.410	2789	2792	2799	rBV2	1567	2100	0.24%	0.036%
27	19.522	2805	2811	2819	rBV	328869	444774	51.23%	7.603%
28	19.857	2866	2868	2871	rBV	787	908	0.10%	0.016%
29	20.057	2899	2902	2904	rBV	2299	2029	0.23%	0.035%
30	20.339	2946	2950	2952	rBV3	816	1079	0.12%	0.018%
31	20.557	2984	2987	2989	rVV2	5502	5196	0.60%	0.089%
32	21.022	3062	3066	3070	rBV	14395	17178	1.98%	0.294%
33	21.098	3076	3079	3084	rBV2	4347	5566	0.64%	0.095%
34	21.228	3098	3101	3104	rBV3	4246	5355	0.62%	0.092%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004504.D
Acq On : 26 Feb 2019 18:22
Operator : JU/SJ
Sample : K1553-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5X2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION

35	21.322	3111	3117	3125	rBV	589318	698750	80.48%	11.944%
36	21.463	3137	3141	3144	rVB	13738	15858	1.83%	0.271%
37	21.898	3211	3215	3224	rVB	20100	26978	3.11%	0.461%
38	22.363	3290	3294	3303	rVB	29424	36677	4.22%	0.627%
39	22.492	3313	3316	3323	rVB	19374	23318	2.69%	0.399%
40	22.875	3377	3381	3388	rVB	32828	47859	5.51%	0.818%
41	23.445	3470	3478	3487	rBV	405124	743082	85.58%	12.702%
42	23.586	3495	3502	3514	rVB2	455557	868263	100.00%	14.841%
43	24.092	3584	3588	3596	rVB	35375	72596	8.36%	1.241%
44	24.851	3711	3717	3728	rVB	36047	79874	9.20%	1.365%
45	25.727	3861	3866	3875	rVB2	20468	51734	5.96%	0.884%


Sum of corrected areas: 5850346

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004504.D
Acq On : 26 Feb 2019 18:22
Operator : JU/SJ
Sample : K1553-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5X2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

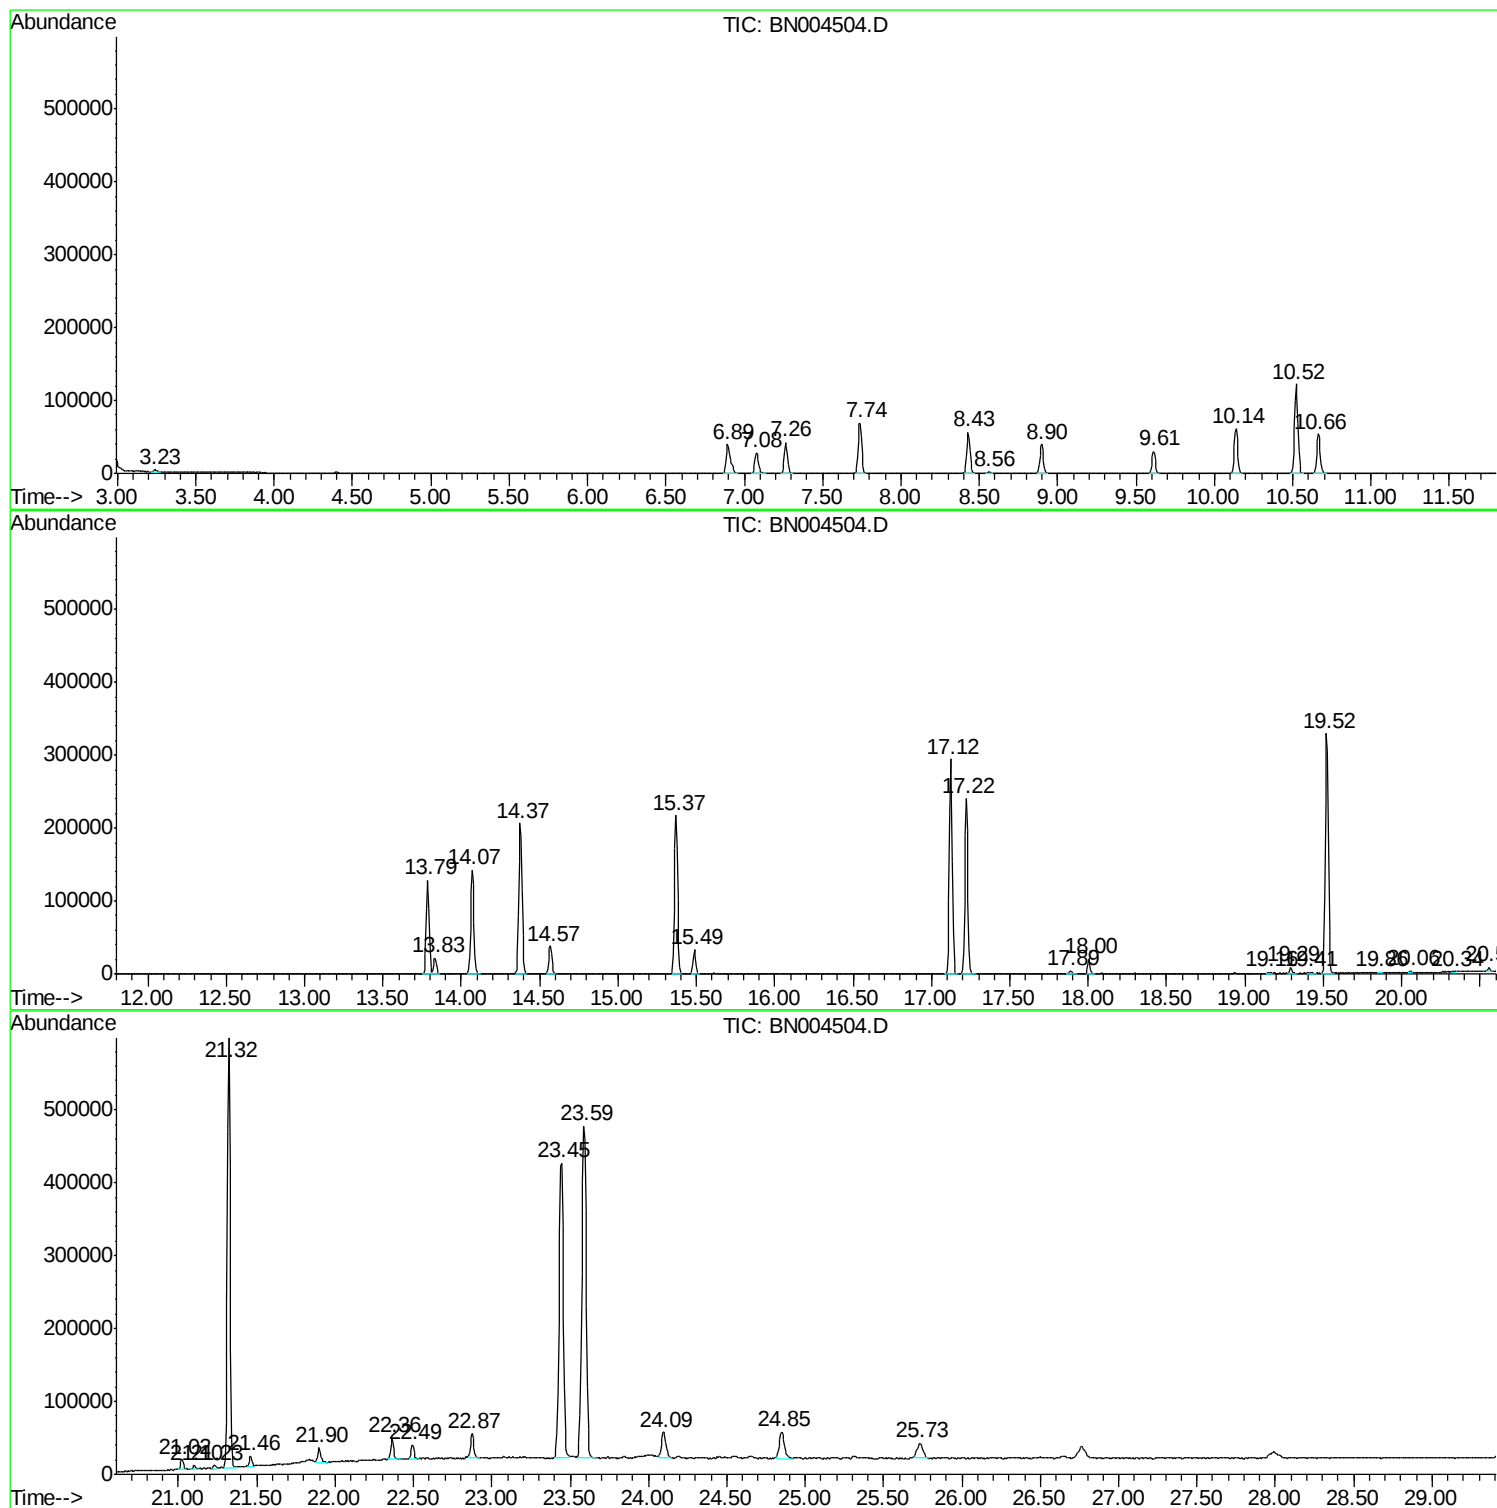

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004504.D
Acq On : 26 Feb 2019 18:22
Operator : JU/SJ
Sample : K1553-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5X2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004504.D
Acq On : 26 Feb 2019 18:22
Operator : JU/SJ
Sample : K1553-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5X2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc