

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022619\
 Data File : BN004514.D
 Acq On : 27 Feb 2019 00:16
 Operator : JU/SJ
 Sample : K1553-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5W9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	50	rVB	4603	6659	0.61%	0.087%
2	3.752	128	130	134	rBV	1689	1817	0.17%	0.024%
3	4.852	315	317	321	rVB2	1502	1620	0.15%	0.021%
4	6.893	659	664	673	rBB	58456	89455	8.19%	1.168%
5	7.075	690	695	704	rBV	40553	61577	5.64%	0.804%
6	7.263	722	727	734	rBB	60253	91033	8.34%	1.188%
7	7.734	802	807	814	rBB	111315	174709	16.00%	2.281%
8	8.428	920	925	931	rBB	77614	114712	10.51%	1.498%
9	8.557	943	947	952	rBB	4728	6897	0.63%	0.090%
10	8.899	999	1005	1011	rBB	54591	85123	7.80%	1.111%
11	9.257	1063	1066	1068	rBB2	1216	1150	0.11%	0.015%
12	9.610	1121	1126	1132	rBB	43453	65044	5.96%	0.849%
13	10.140	1210	1216	1222	rBB	84433	133612	12.24%	1.744%
14	10.522	1274	1281	1288	rBB	184190	299660	27.44%	3.912%
15	10.663	1299	1305	1315	rBB	51459	81732	7.49%	1.067%
16	11.963	1522	1526	1530	rBB	2650	3851	0.35%	0.050%
17	13.787	1830	1836	1840	rBV	165306	219671	20.12%	2.868%
18	13.828	1840	1843	1848	rVB	26662	33894	3.10%	0.442%
19	14.069	1878	1884	1890	rBV	184430	259643	23.78%	3.389%
20	14.375	1930	1936	1943	rBB2	297881	451692	41.37%	5.897%
21	14.569	1964	1969	1975	rBB	56892	74537	6.83%	0.973%
22	15.116	2059	2062	2064	rBB	2062	2002	0.18%	0.026%
23	15.198	2072	2076	2079	rBB	2021	2308	0.21%	0.030%
24	15.369	2099	2105	2111	rBB	268406	368175	33.72%	4.806%
25	15.487	2120	2125	2130	rBB	44923	54662	5.01%	0.714%
26	15.610	2143	2146	2148	rBB	1286	1371	0.13%	0.018%
27	15.745	2166	2169	2171	rBB	1879	1468	0.13%	0.019%
28	16.075	2221	2225	2228	rBB	968	1303	0.12%	0.017%
29	16.910	2364	2367	2370	rBB2	1214	1449	0.13%	0.019%
30	17.122	2397	2403	2409	rBV2	427055	586587	53.72%	7.658%
31	17.222	2414	2420	2427	rBV	292869	395924	36.26%	5.169%
32	18.004	2549	2553	2559	rVB	22675	26291	2.41%	0.343%
33	18.081	2564	2566	2570	rVB2	936	1176	0.11%	0.015%
34	19.151	2745	2748	2752	rBV	2417	3065	0.28%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
 Data File : BN004514.D
 Acq On : 27 Feb 2019 00:16
 Operator : JU/SJ
 Sample : K1553-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5W9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION

35	19.186	2752	2754	2757	rVB	1070	1240	0.11%	0.016%
36	19.292	2769	2772	2776	rBV	7385	8657	0.79%	0.113%
37	19.410	2789	2792	2795	rVB	1473	1851	0.17%	0.024%
38	19.522	2805	2811	2820	rBV	404294	525590	48.13%	6.861%
39	20.057	2895	2902	2905	rBV2	3396	4043	0.37%	0.053%
40	20.551	2983	2986	2991	rBV	6424	7908	0.72%	0.103%
41	21.022	3061	3066	3070	rBV2	27365	35943	3.29%	0.469%
42	21.227	3097	3101	3106	rBV2	7807	9154	0.84%	0.120%
43	21.322	3111	3117	3130	rVV	763599	975119	89.30%	12.730%
44	21.457	3136	3140	3145	rBV	19385	21952	2.01%	0.287%
45	21.821	3200	3202	3210	rVB5	7281	9446	0.87%	0.123%
46	21.892	3210	3214	3221	rBV	25540	34933	3.20%	0.456%
47	21.974	3225	3228	3233	rVB2	9733	12158	1.11%	0.159%
48	22.363	3290	3294	3299	rVB	40160	50229	4.60%	0.656%
49	22.492	3312	3316	3322	rVB	17283	23138	2.12%	0.302%
50	22.868	3376	3380	3389	rVB	51824	78697	7.21%	1.027%
51	23.439	3470	3477	3485	rBV	438295	812781	74.43%	10.610%
52	23.586	3495	3502	3510	rVB	592402	1091939	100.00%	14.255%
53	24.092	3583	3588	3596	rVB	50527	96772	8.86%	1.263%
54	24.845	3711	3716	3725	rVB	45291	94605	8.66%	1.235%
55	25.727	3861	3866	3874	rVB3	24891	60196	5.51%	0.786%


Sum of corrected areas: 7660220

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022619\
Data File : BN004514.D
Acq On : 27 Feb 2019 00:16
Operator : JU/SJ
Sample : K1553-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5W9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

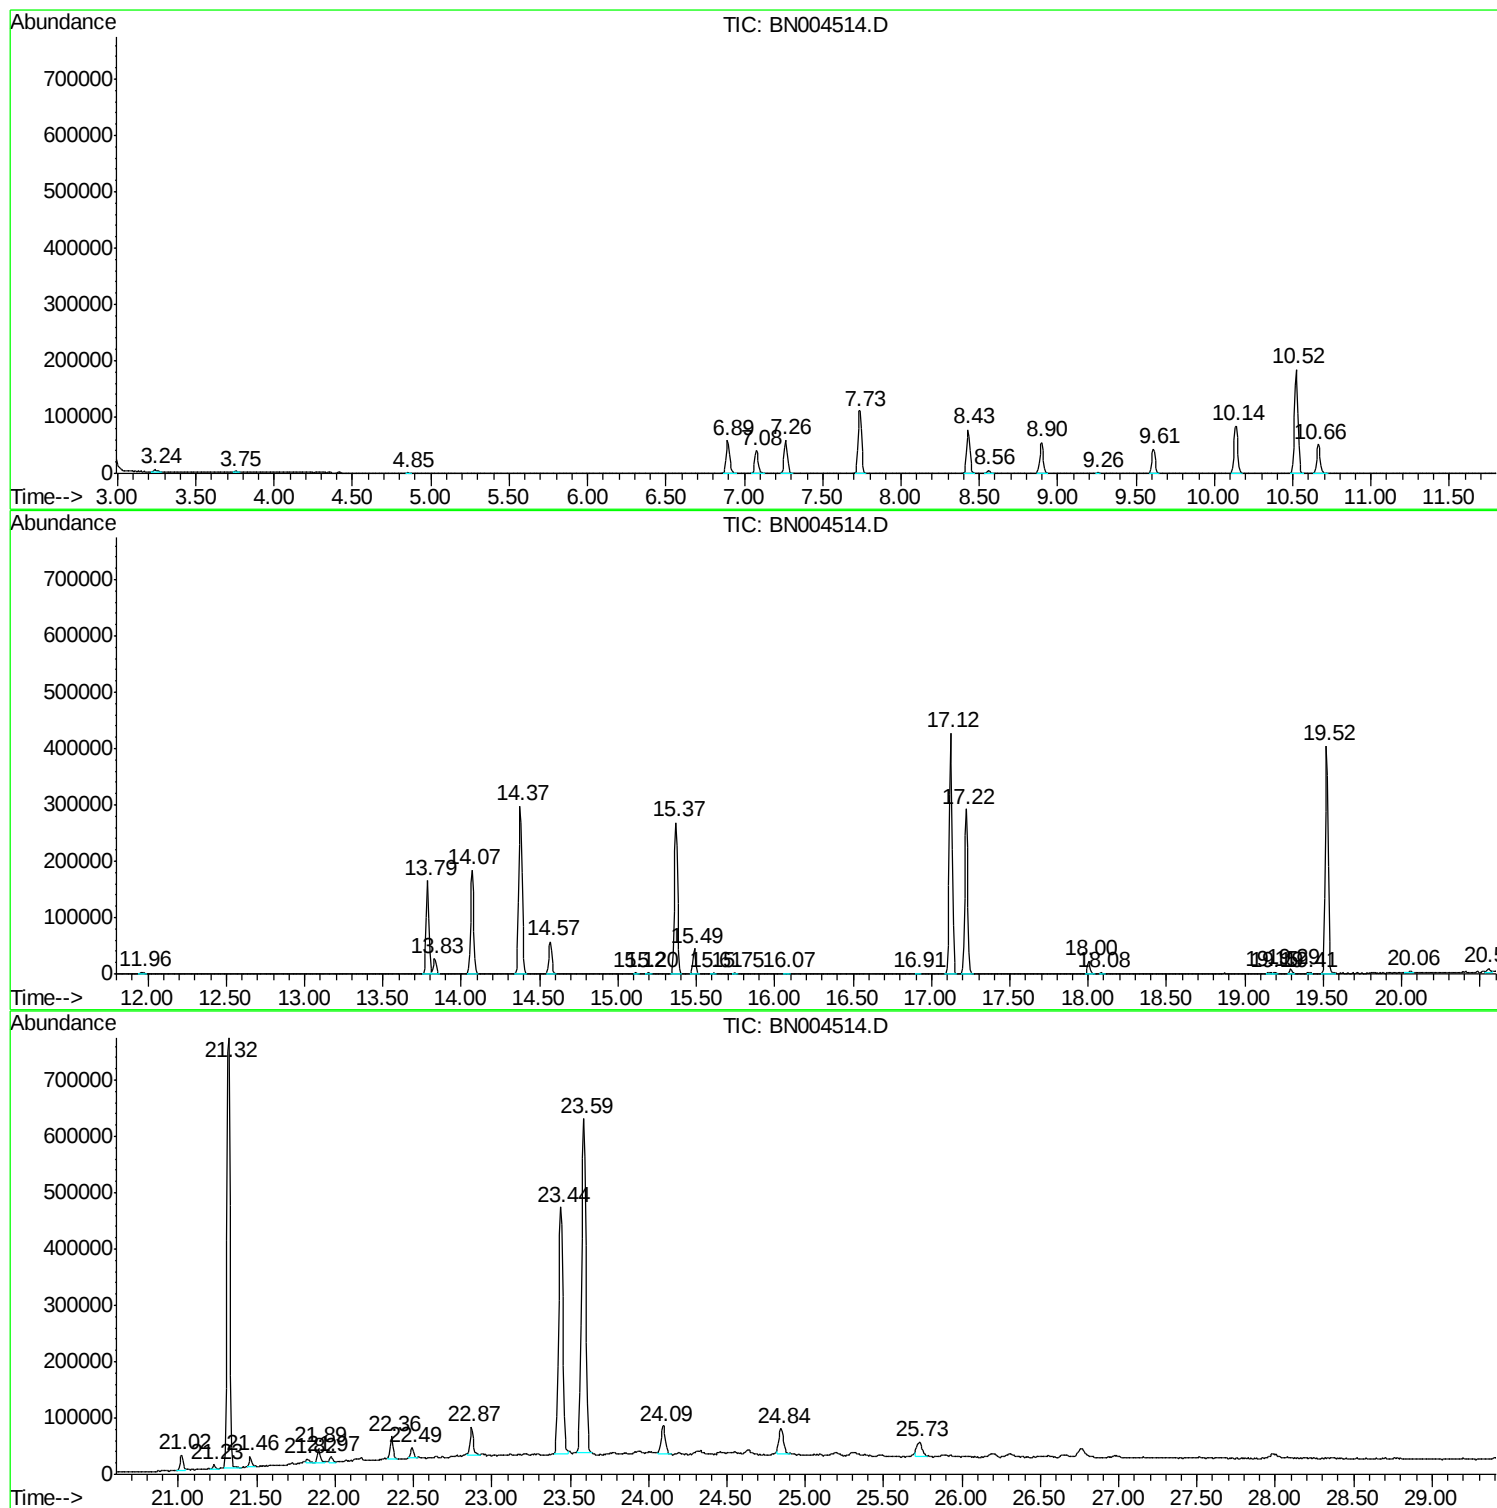

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004514.D
Acq On : 27 Feb 2019 00:16
Operator : JU/SJ
Sample : K1553-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5W9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022619\
Data File : BN004514.D
Acq On : 27 Feb 2019 00:16
Operator : JU/SJ
Sample : K1553-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5W9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
