

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022719\
 Data File : BN004543.D
 Acq On : 28 Feb 2019 01:11
 Operator : JU/SJ
 Sample : K1600-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF7Y9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	48	rVB	6727	9166	0.49%	0.067%
2	4.475	250	253	258	rVB	4583	5372	0.29%	0.039%
3	6.893	659	664	672	rBB	38643	60563	3.25%	0.441%
4	7.075	689	695	709	rBB	103029	164027	8.81%	1.194%
5	7.263	721	727	734	rBB	129534	197357	10.60%	1.437%
6	7.734	801	807	814	rBB	170149	258680	13.90%	1.883%
7	8.428	919	925	931	rBB	105931	157310	8.45%	1.145%
8	8.893	998	1004	1012	rBB	138004	219349	11.78%	1.597%
9	9.251	1061	1065	1069	rBB2	5801	8085	0.43%	0.059%
10	9.610	1120	1126	1132	rBB	116047	189852	10.20%	1.382%
11	10.134	1209	1215	1222	rBB	216419	339078	18.22%	2.468%
12	10.516	1274	1280	1288	rBB	277151	441955	23.74%	3.217%
13	10.663	1300	1305	1310	rBB	6925	10750	0.58%	0.078%
14	12.104	1547	1550	1554	rBB	2722	3735	0.20%	0.027%
15	13.781	1829	1835	1841	rBV	442699	596851	32.07%	4.345%
16	14.069	1877	1884	1890	rBV	506748	760284	40.85%	5.535%
17	14.375	1930	1936	1943	rBB2	431777	640647	34.42%	4.664%
18	14.569	1964	1969	1974	rBB	52129	62530	3.36%	0.455%
19	15.369	2099	2105	2111	rBV	690011	948706	50.97%	6.906%
20	15.486	2120	2125	2131	rBB	224850	266859	14.34%	1.943%
21	15.604	2141	2145	2149	rBB	4897	5932	0.32%	0.043%
22	17.122	2397	2403	2409	rBV	597920	810596	43.55%	5.901%
23	17.222	2412	2420	2428	rBV2	782776	1094457	58.80%	7.967%
24	17.875	2528	2531	2535	rBB2	4831	5170	0.28%	0.038%
25	18.004	2549	2553	2564	rVB	43987	58652	3.15%	0.427%
26	18.351	2605	2612	2614	rBV2	1641	2369	0.13%	0.017%
27	19.157	2744	2749	2757	rVB2	9825	16296	0.88%	0.119%
28	19.292	2768	2772	2778	rBV	21900	27835	1.50%	0.203%
29	19.410	2788	2792	2795	rBV	6845	9392	0.50%	0.068%
30	19.521	2805	2811	2819	rBV2	1032218	1424502	76.53%	10.370%
31	20.057	2900	2902	2905	rVB2	1930	2033	0.11%	0.015%
32	20.339	2947	2950	2952	rBV3	1340	1880	0.10%	0.014%
33	20.498	2975	2977	2980	rVB3	2223	1907	0.10%	0.014%
34	20.551	2983	2986	2990	rVV3	3864	4451	0.24%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022719\
Data File : BN004543.D
Acq On : 28 Feb 2019 01:11
Operator : JU/SJ
Sample : K1600-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF7Y9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION

35	21.016	3061	3065	3069	rBV3	13987	17699	0.95%	0.129%
36	21.221	3097	3100	3107	rVB	8088	10574	0.57%	0.077%
37	21.316	3111	3116	3122	rBV	938393	1210239	65.02%	8.810%
38	21.457	3137	3140	3145	rBV	14440	13982	0.75%	0.102%
39	21.892	3211	3214	3220	rVB	30335	34622	1.86%	0.252%
40	22.357	3289	3293	3304	rVB	50994	72745	3.91%	0.530%
41	22.486	3312	3315	3319	rBV	12019	14812	0.80%	0.108%
42	22.868	3376	3380	3387	rVB	63386	86960	4.67%	0.633%
43	23.439	3469	3477	3491	rVB2	1032566	1861316	100.00%	13.550%
44	23.580	3494	3501	3512	rVB2	678772	1278674	68.70%	9.308%
45	24.092	3582	3588	3595	rVB	58627	114482	6.15%	0.833%
46	24.439	3645	3647	3652	rVB5	5741	8608	0.46%	0.063%
47	24.845	3709	3716	3727	rVB	54900	124259	6.68%	0.905%
48	25.721	3858	3865	3878	rVB2	31652	81079	4.36%	0.590%


Sum of corrected areas: 13736679

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022719\
Data File : BN004543.D
Acq On : 28 Feb 2019 01:11
Operator : JU/SJ
Sample : K1600-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF7Y9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

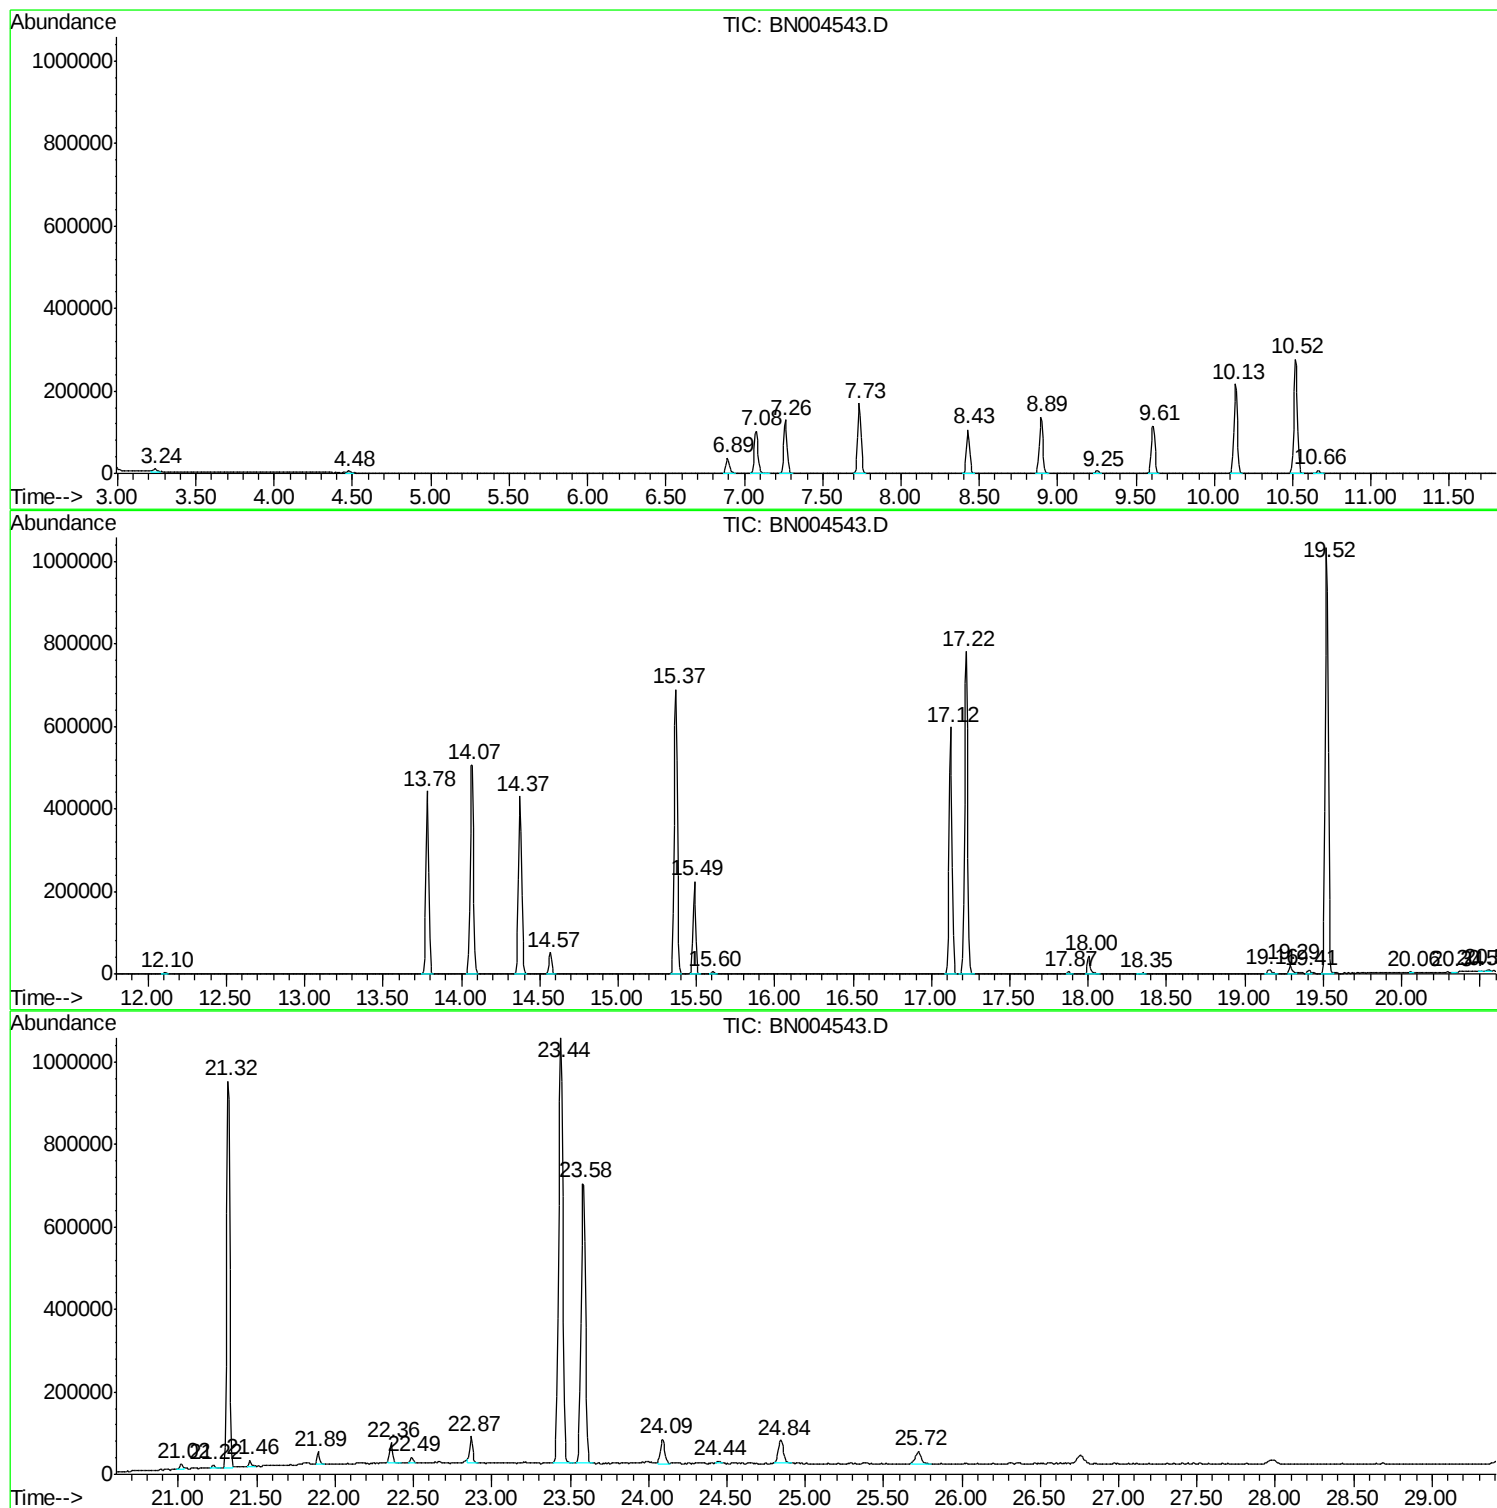

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022719\
Data File : BN004543.D
Acq On : 28 Feb 2019 01:11
Operator : JU/SJ
Sample : K1600-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF7Y9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022719\
Data File : BN004543.D
Acq On : 28 Feb 2019 01:11
Operator : JU/SJ
Sample : K1600-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF7Y9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc