

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030119\
 Data File : BN004575.D
 Acq On : 01 Mar 2019 13:54
 Operator : JU/SJ
 Sample : K1601-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF7X8

Quant Time: Mar 02 03:57:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 02 03:55:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	25893	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.52	136	126507	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	82475	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	202003	20.00	ng/ul	-0.02
78) Chrysene-d12	21.32	240	257665	20.00	ng/ul	-0.01
86) Perylene-d12	23.58	264	291970	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	1079	2.51	ng/uL	-0.01
5) Phenol-d5	6.89	99	30474	13.21	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	18836	16.27	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	27418	14.65	ng/ul	-0.02
13) 4-Methylphenol-d8	8.42	113	27621	13.93	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	13784	16.46	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	15413	17.63	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	29206	14.74	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	43135	19.68	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	118924	17.00	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	126210	15.23	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.56	143	15873	11.85	ng/ul	-0.02
58) Fluorene-d10	15.36	176	100704	16.36	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.48	200	13906	11.80	ng/ul	-0.02
71) Anthracene-d10	17.22	188	156208	16.14	ng/ul	-0.02
79) Pyrene-d10	19.52	212	190047	16.46	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.43	264	245730	16.04	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.83	163	15483	2.239	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030119\
Data File : BN004575.D
Acq On : 01 Mar 2019 13:54
Operator : JU/SJ
Sample : K1601-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF7X8

Quant Time: Mar 02 03:57:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 02 03:55:03 2019
Response via : Initial Calibration

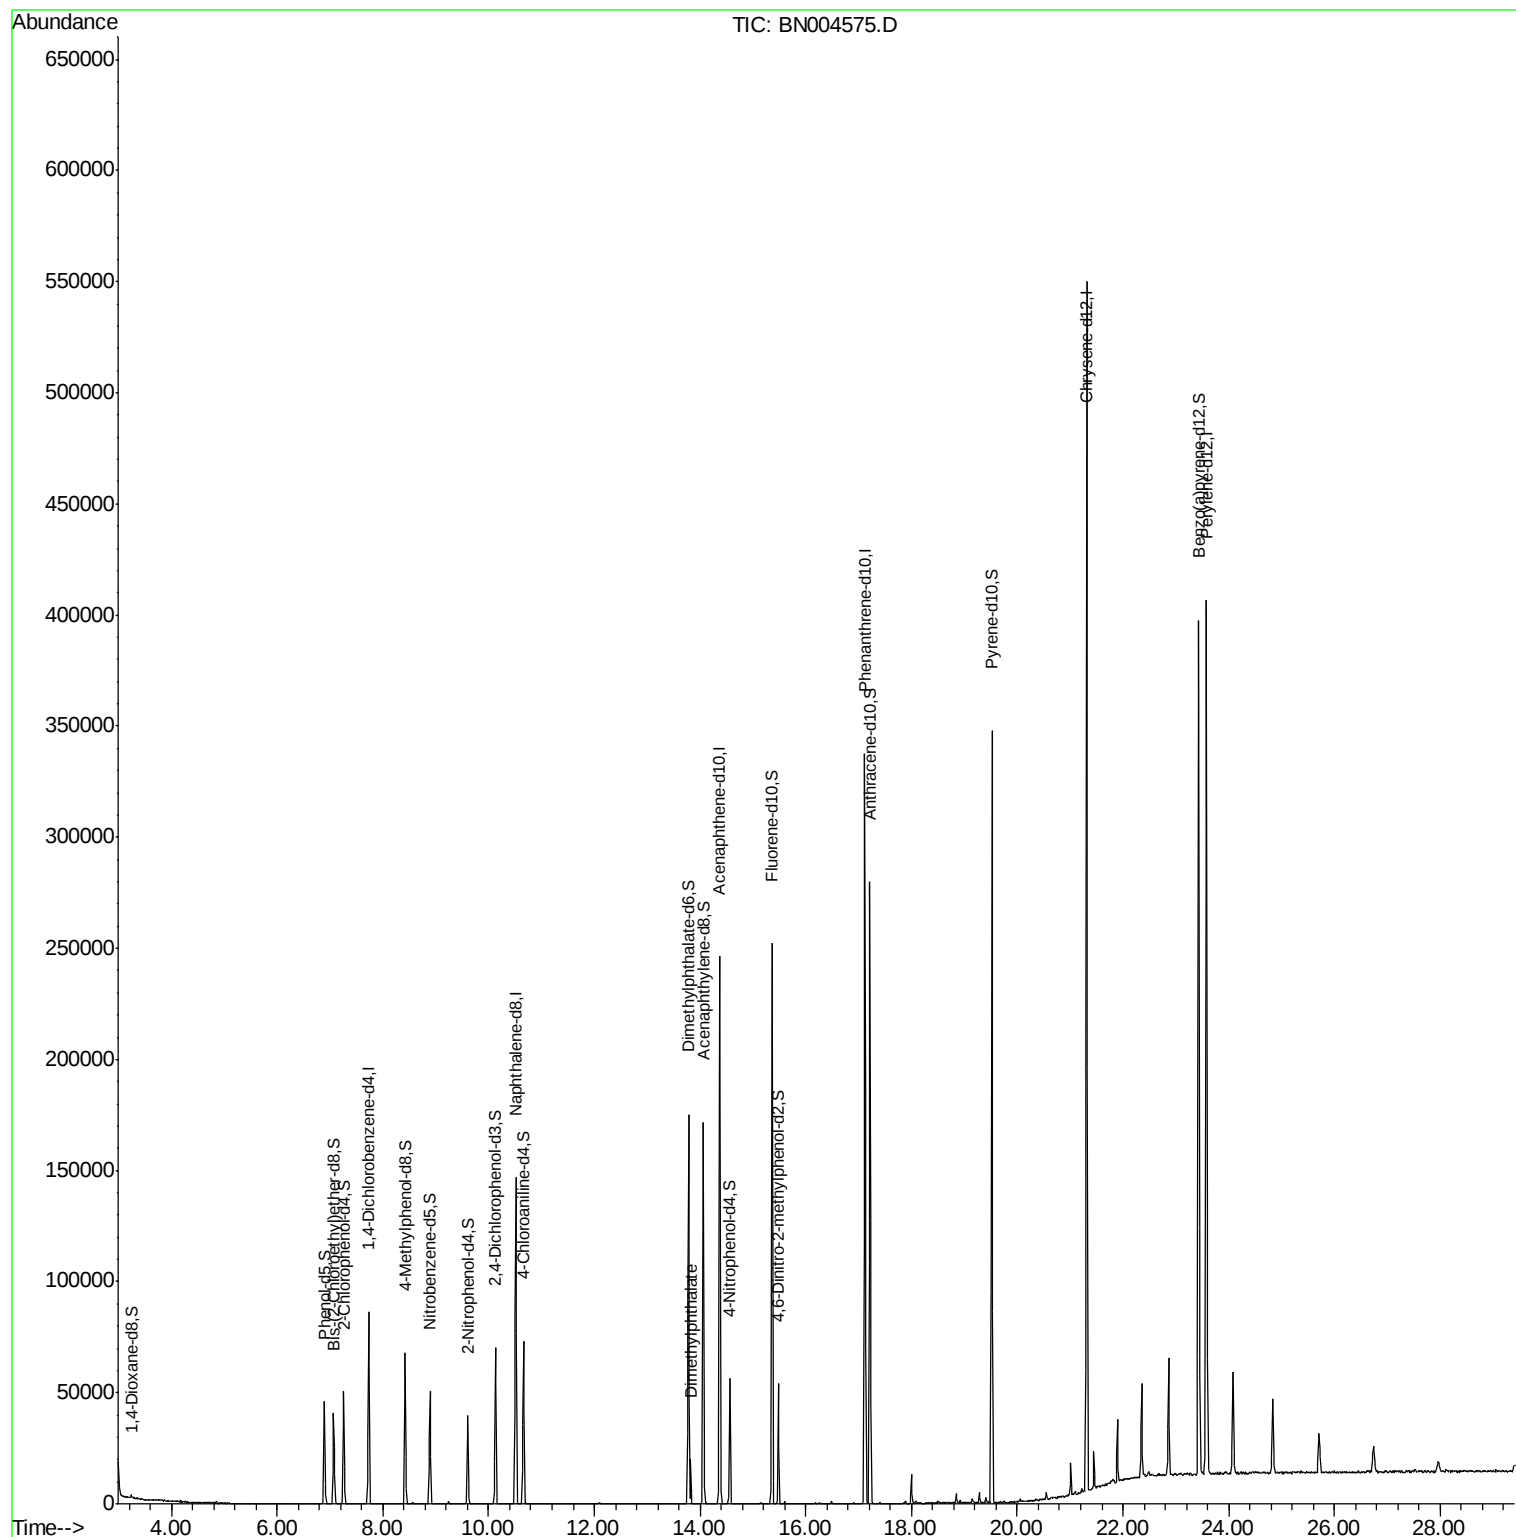

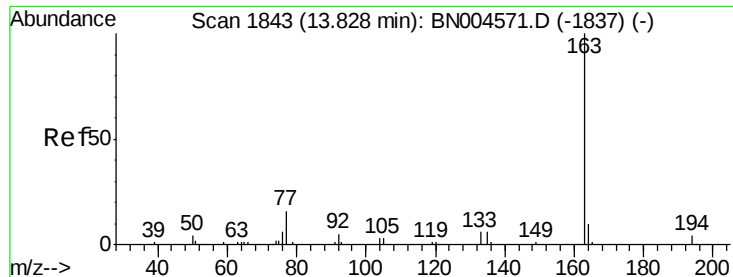

#45

Dimethylphthalate

Concen: 2.239 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004575.D


Acq: 01 Mar 2019 13:54

Instrument :

BNA_N

ClientSampleId :

BF7X8

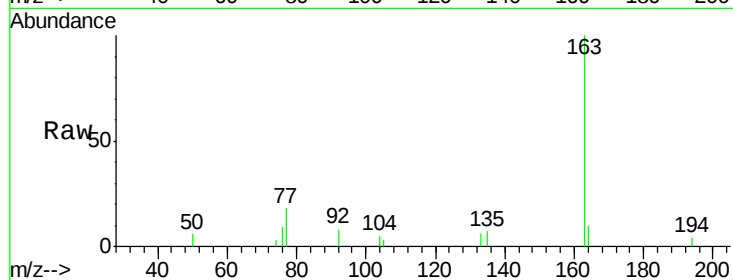


Tgt Ion:163 Resp: 15483

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.4 7.9 11.9

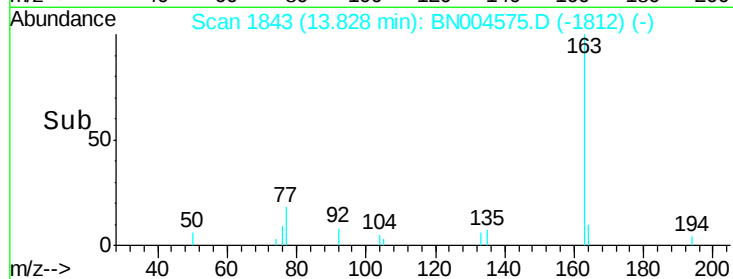

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

