

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030119\
 Data File : BN004577.D
 Acq On : 01 Mar 2019 15:04
 Operator : JU/SJ
 Sample : K1601-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF7Y0

Quant Time: Mar 02 03:57:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 02 03:55:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	28698	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.52	136	141730	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	90040	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	217856	20.00	ng/ul	-0.02
78) Chrysene-d12	21.32	240	278668	20.00	ng/ul	-0.01
86) Perylene-d12	23.58	264	311890	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	2780	5.82	ng/uL	-0.01
5) Phenol-d5	6.89	99	29214	11.42	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	18229	14.20	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	27477	13.25	ng/ul	-0.02
13) 4-Methylphenol-d8	8.42	113	24760	11.26	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	13767	14.67	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	15230	15.55	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	29702	13.38	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	36118	14.71	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	112927	14.79	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	123495	13.65	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.56	143	16048	10.98	ng/ul	-0.02
58) Fluorene-d10	15.36	176	99273	14.77	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.49	200	13701	10.78	ng/ul	-0.01
71) Anthracene-d10	17.22	188	153093	14.66	ng/ul	-0.02
79) Pyrene-d10	19.52	212	185072	14.82	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.43	264	232240	14.19	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.83	163	14089	1.866	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030119\
Data File : BN004577.D
Acq On : 01 Mar 2019 15:04
Operator : JU/SJ
Sample : K1601-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF7Y0

Quant Time: Mar 02 03:57:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 02 03:55:03 2019
Response via : Initial Calibration

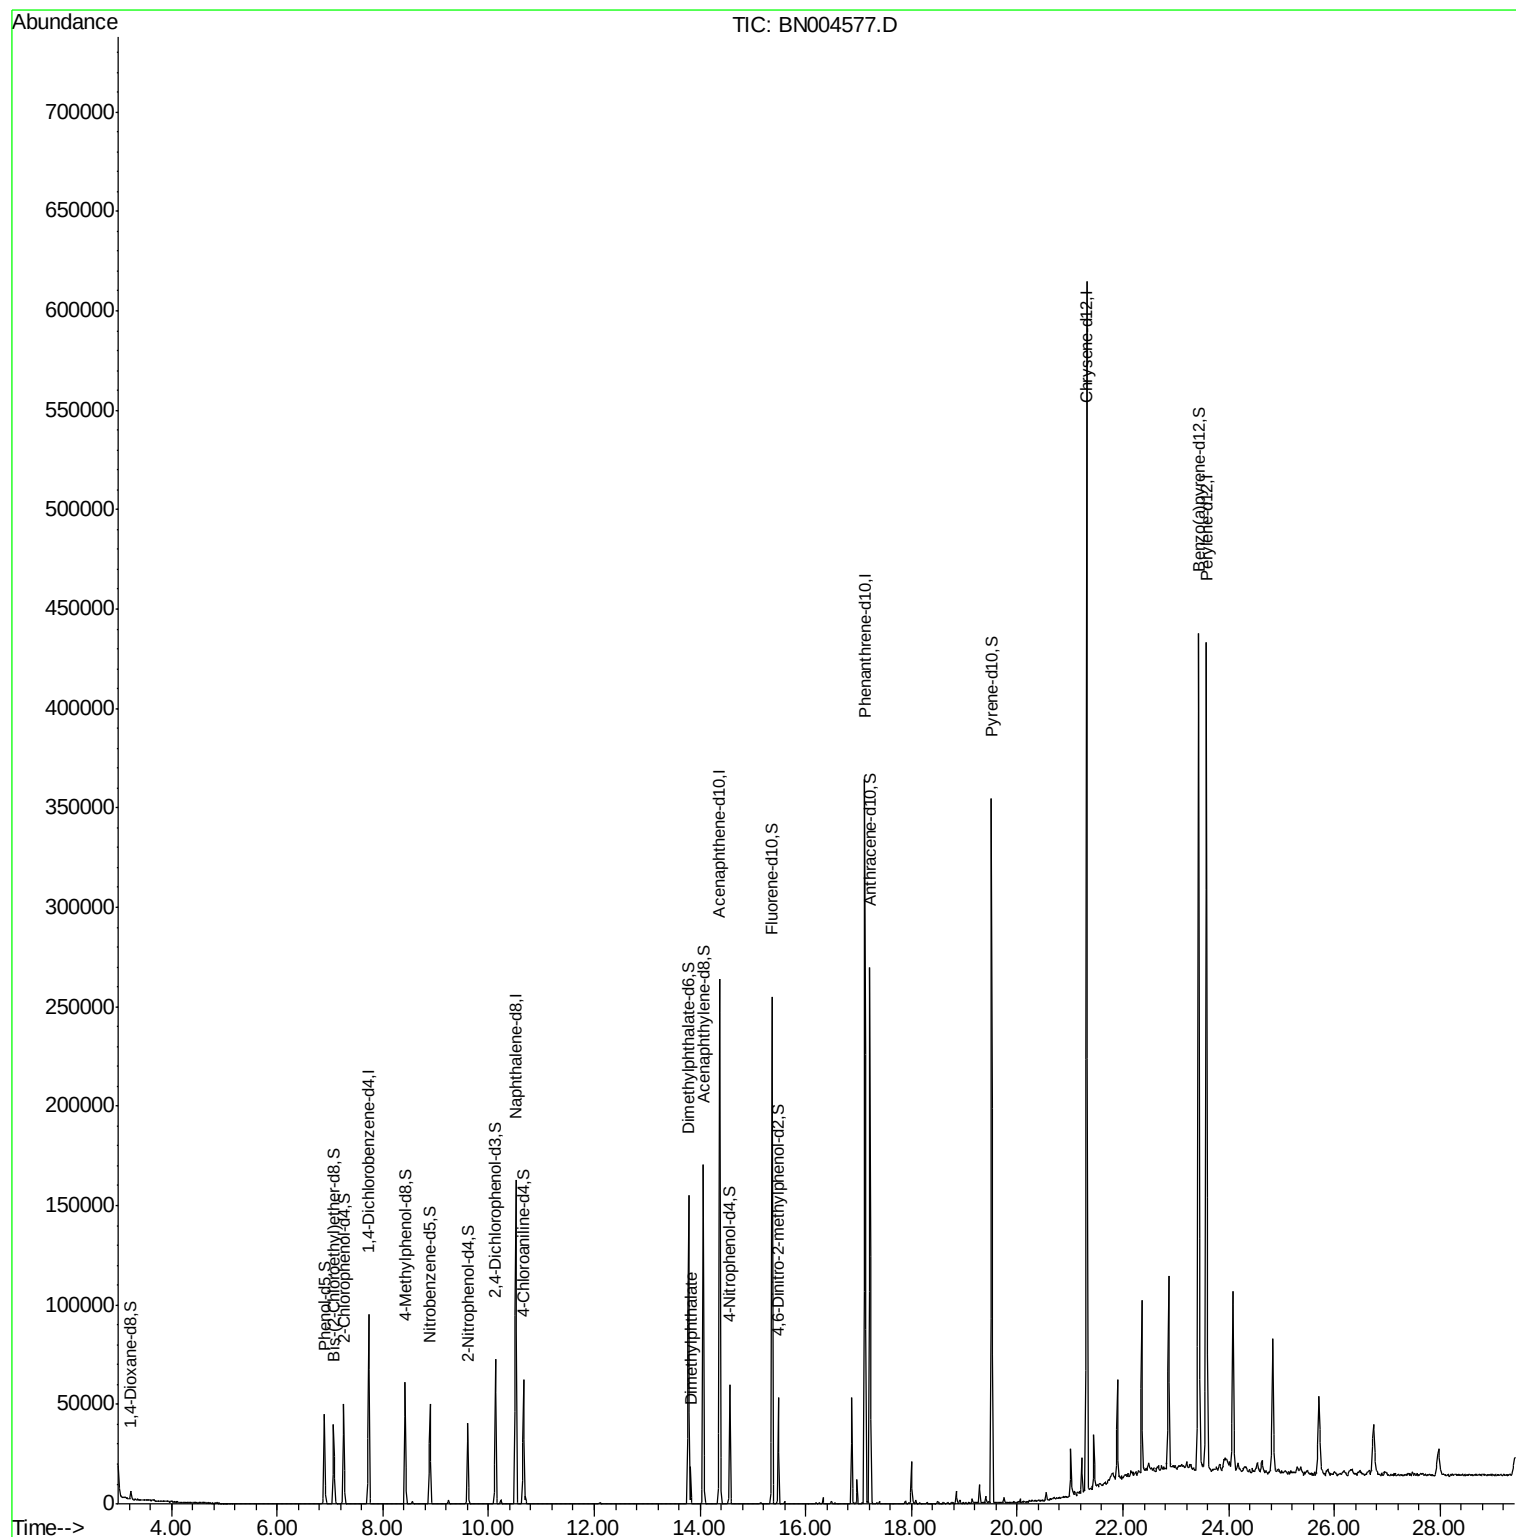

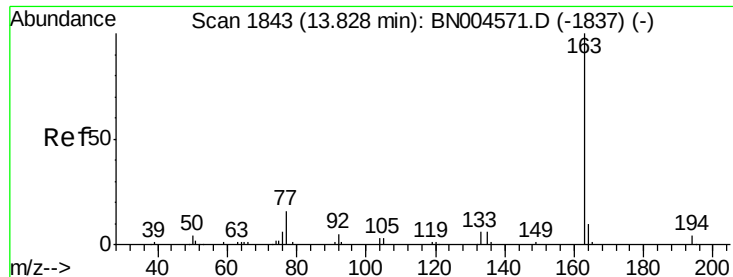

#45

Dimethylphthalate

Concen: 1.866 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004577.D


Acq: 01 Mar 2019 15:04

Instrument :

BNA_N

ClientSampleId :

BF7Y0

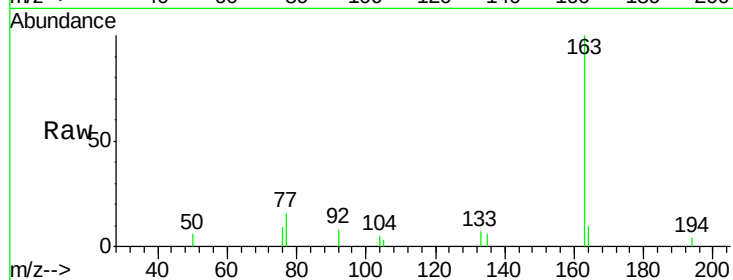


Tgt Ion:163 Resp: 14089

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 9.6 7.9 11.9

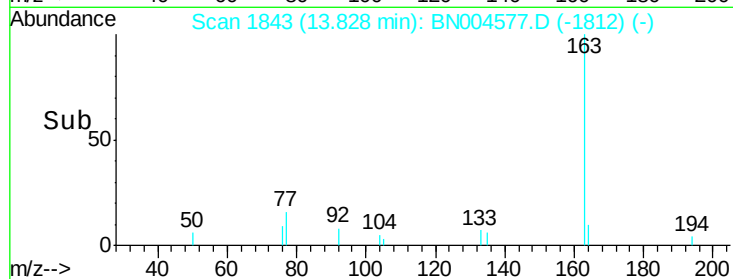

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

