


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030119\
Data File : BN004570.D
Acq On : 01 Mar 2019 10:50
Operator : JU/SJ
Sample : DFTPP12
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP12

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION
Last Update : Mon Mar 04 03:57:45 2019

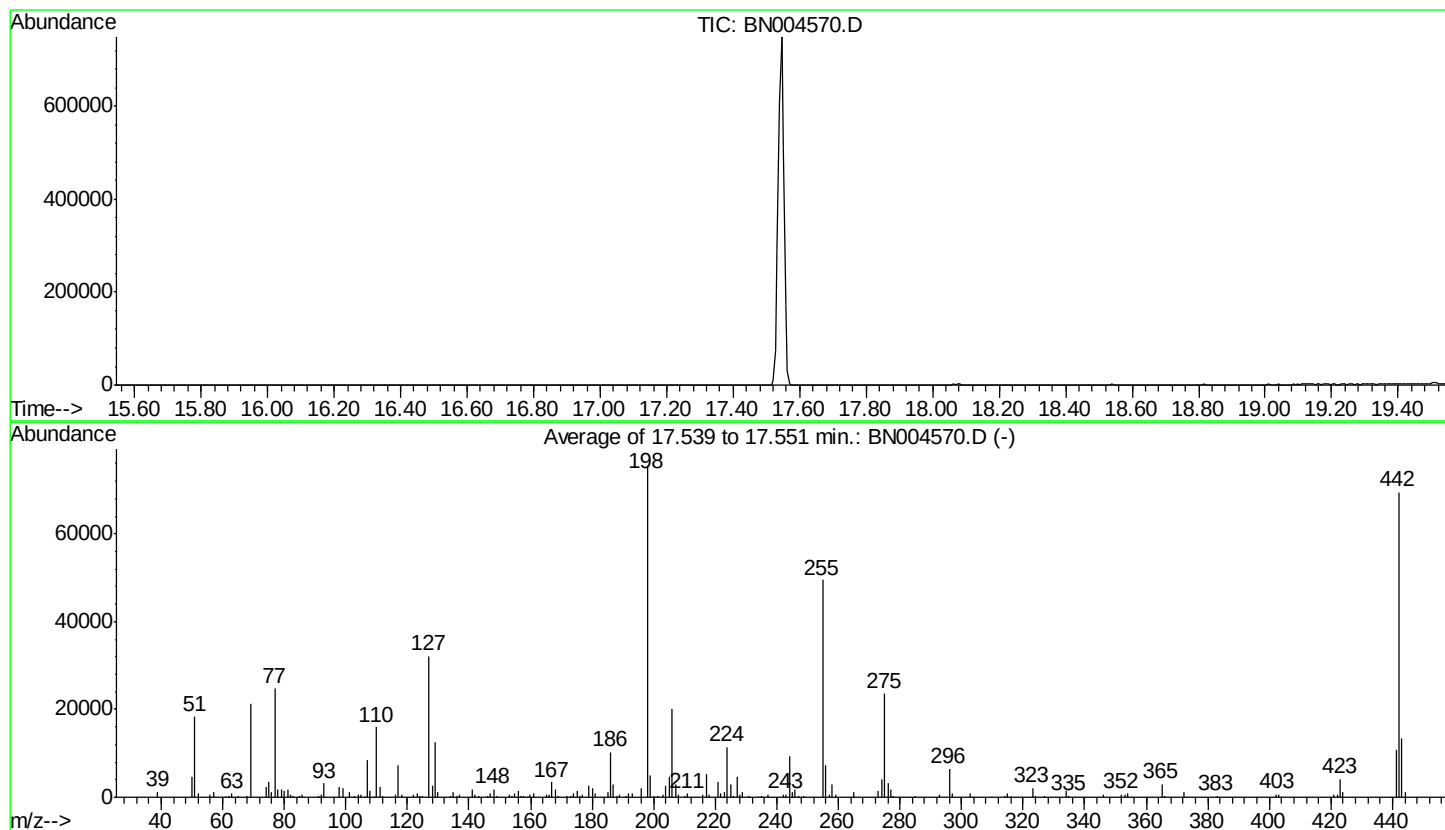

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.3	18343	PASS
68	69	0.00	2	1.5	313	PASS
69	198	0.00	100	28.1	21196	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	32192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75541	PASS
199	198	5	9	6.7	5065	PASS
275	198	10	60	31.2	23560	PASS
365	198	1	100	4.0	3025	PASS
441	198	0.01	100	14.3	10781	PASS
442	198	50	100	92.0	69480	PASS
443	442	15	24	19.2	13324	PASS

m/z	Abundance
39.00	1376.0
40.00	640.0
50.00	5401.0
51.00	21064.0
52.00	1095.0
56.00	629.0
57.00	1463.0
61.00	309.0
62.00	319.0
63.00	921.0
65.00	499.0
68.00	435.0
69.00	23384.0
74.00	2435.0
75.00	3833.0
76.00	1343.0
77.00	27480.0
78.00	1938.0
79.00	1948.0
80.00	1408.0
81.00	2018.0
81.90	474.0
83.00	451.0
84.90	364.0
86.00	553.0
91.00	476.0
92.00	538.0
93.00	3597.0
98.00	2647.0
99.00	2272.0
101.00	1166.0
103.00	395.0
104.00	759.0
105.00	713.0
107.00	9304.0
108.00	1455.0
110.00	17232.0
111.00	2663.0
111.90	312.0
116.00	516.0
117.00	7789.0
118.00	594.0
121.90	676.0
123.00	947.0
124.00	487.0
125.00	420.0
127.00	34776.0
128.00	2729.0
129.00	13361.0
130.00	1175.0
134.00	379.0
135.00	1104.0
135.90	432.0
137.00	549.0
141.00	1747.0
142.00	575.0
143.00	419.0
146.00	323.0
147.00	911.0
148.00	1983.0
148.90	487.0
153.00	609.0
154.00	394.0
155.00	938.0
156.00	1456.0
157.10	303.0
157.90	315.0
159.90	509.0
161.00	805.0
165.00	681.0
165.90	546.0
167.00	3492.0
168.00	2038.0
169.00	357.0
171.90	314.0
173.00	418.0
174.00	800.0
175.00	1420.0
176.00	406.0
176.90	691.0
179.00	2724.0
180.00	1996.0
181.00	839.0
185.00	1288.0
186.00	10235.0
187.00	2982.0
188.00	350.0
189.00	692.0
191.00	333.0
192.00	824.0
193.00	954.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12

196.00	2222.0
198.00	74640.0
199.00	5180.0
200.00	447.0
201.50	393.0
202.90	573.0
204.00	2683.0
205.00	4572.0
206.00	19808.0
207.00	2840.0
208.00	713.0
210.20	325.0
211.00	798.0
216.00	438.0
217.00	5265.0
218.00	717.0
221.00	3175.0
221.80	766.0
223.00	1204.0
224.00	11165.0
225.00	2904.0
226.10	353.0
227.00	4550.0
227.90	653.0
229.00	992.0
231.00	374.0
234.90	340.0
237.00	466.0
242.00	580.0
243.00	592.0
244.00	8770.0
245.00	1302.0
246.00	1706.0
246.90	385.0
248.90	369.0
255.00	46656.0
256.00	7076.0
257.00	627.0
258.00	2697.0
258.90	490.0
265.00	1066.0
273.00	1440.0
274.00	3639.0
275.00	21616.0
276.00	2980.0
277.00	1822.0
278.00	338.0
285.00	313.0
293.00	414.0
296.00	5813.0
297.00	810.0
303.00	730.0
314.00	309.0
315.00	642.0
316.00	394.0
323.00	1911.0
324.00	383.0
326.90	394.0
334.00	1280.0
335.00	330.0
345.90	365.0
352.00	577.0
353.00	408.0
354.00	653.0
365.00	2560.0
365.90	368.0
372.00	1073.0
382.90	306.0
402.00	390.0
402.90	587.0
421.00	485.0
422.00	493.0
423.00	3315.0
424.00	1050.0
441.10	8334.0
442.00	53320.0
443.00	10318.0
444.00	980.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12

m/z	Abundance
39.00	1505.0
39.90	703.0
50.00	5385.0
51.00	21408.0
52.00	1094.0
56.00	609.0
57.00	1494.0
62.00	318.0
63.00	896.0
65.00	511.0
68.00	506.0
69.00	25344.0
74.00	2697.0
75.00	4087.0
76.00	1408.0
77.00	29136.0
78.00	2035.0
79.00	2067.0
80.00	1642.0
81.00	2237.0
81.90	570.0
83.00	466.0
85.00	471.0
86.00	629.0
91.00	530.0
92.00	624.0
93.00	3566.0
98.00	2867.0
99.00	2328.0
101.00	1310.0
102.90	400.0
104.00	877.0
105.00	789.0
106.10	310.0
107.00	10160.0
108.00	1637.0
109.10	329.0
110.00	18864.0
111.00	2879.0
111.90	330.0
116.00	589.0
117.00	8507.0
118.00	585.0
122.00	691.0
123.00	1158.0
124.00	529.0
125.00	427.0
127.00	38040.0
128.00	2957.0
129.00	14940.0
130.00	1277.0
133.90	453.0
135.00	1305.0
136.00	538.0
137.00	712.0
141.00	1920.0
142.00	695.0
142.90	485.0
145.90	357.0
147.00	1071.0
148.00	2231.0
149.00	467.0
153.00	624.0
153.90	517.0
155.00	1122.0
156.00	1771.0
157.00	339.0
157.90	410.0
159.00	316.0
160.00	665.0
161.00	938.0
165.00	774.0
165.90	617.0
167.00	4121.0
168.00	2186.0
169.00	367.0
171.90	433.0
173.00	491.0
174.00	889.0
175.00	1675.0
176.00	443.0
177.00	829.0
179.00	3208.0
180.00	2310.0
181.00	1001.0
185.00	1513.0
186.00	12451.0
187.00	3510.0
188.00	441.0
189.00	739.0
191.00	354.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12

192.00	1052.0
193.00	1200.0
196.00	2601.0
198.00	91344.0
199.00	6086.0
200.00	490.0
201.50	414.0
203.00	633.0
204.00	3346.0
205.00	5630.0
206.00	24664.0
207.00	3468.0
208.00	867.0
210.20	368.0
211.00	981.0
216.00	537.0
217.00	6384.0
218.00	890.0
221.00	4146.0
221.80	965.0
223.00	1430.0
224.00	13795.0
225.00	3768.0
226.00	445.0
227.00	5708.0
228.00	843.0
229.00	1287.0
231.00	517.0
233.90	333.0
235.00	398.0
237.00	548.0
242.00	674.0
243.10	794.0
244.00	11264.0
245.00	1500.0
246.00	2212.0
246.90	475.0
248.90	431.0
255.00	59328.0
256.00	8747.0
257.00	643.0
258.00	3260.0
259.00	500.0
265.00	1372.0
273.00	1792.0
274.00	4813.0
275.00	28576.0
276.00	3756.0
277.00	2290.0
277.90	380.0
285.00	383.0
293.00	575.0
296.00	7821.0
297.00	1079.0
303.00	785.0
313.90	407.0
315.00	892.0
316.00	501.0
323.00	2567.0
324.00	485.0
326.90	509.0
334.00	1786.0
335.00	482.0
346.00	572.0
352.00	817.0
353.00	495.0
354.10	916.0
365.00	3653.0
366.00	490.0
372.00	1476.0
373.10	423.0
383.00	401.0
402.00	537.0
403.00	883.0
404.00	379.0
420.90	732.0
422.00	657.0
423.00	5037.0
424.00	1305.0
441.10	13056.0
442.00	83136.0
443.10	16251.0
444.00	1597.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12

m/z	Abundance
39.00	883.0
40.00	711.0
50.00	3246.0
51.00	12558.0
52.00	673.0
55.90	392.0
57.00	938.0
63.00	562.0
69.00	14860.0
74.00	1564.0
75.00	2541.0
76.00	886.0
77.00	17440.0
78.00	1197.0
79.00	1297.0
80.00	961.0
81.00	1242.0
81.90	327.0
83.00	306.0
85.90	405.0
92.00	346.0
93.00	2242.0
98.00	1717.0
99.00	1472.0
101.00	797.0
103.90	498.0
104.90	467.0
107.00	6243.0
108.00	983.0
110.00	11797.0
111.00	1723.0
115.90	346.0
117.00	5182.0
117.90	387.0
121.90	443.0
123.00	676.0
125.00	301.0
127.00	23760.0
128.00	1797.0
129.00	9097.0
130.00	762.0
135.00	795.0
135.90	312.0
137.00	393.0
141.00	1303.0
142.00	422.0
147.00	625.0
148.00	1416.0
149.00	312.0
152.90	443.0
155.00	730.0
156.00	1099.0
159.90	439.0
160.90	678.0
165.00	501.0
166.00	382.0
167.00	2541.0
168.00	1431.0
172.90	353.0
174.00	632.0
175.00	1111.0
176.90	646.0
178.90	2046.0
180.00	1536.0
181.00	645.0
185.00	1002.0
186.00	8088.0
187.00	2336.0
189.00	556.0
192.00	763.0
193.00	830.0
196.00	1655.0
198.00	60640.0
199.00	3930.0
202.90	412.0
204.00	2151.0
205.00	3725.0
206.10	16343.0
207.00	2198.0
208.00	550.0
211.00	690.0
216.00	385.0
217.00	4192.0
218.00	555.0
221.00	2816.0
221.80	624.0
222.90	991.0
224.00	9598.0
225.00	2452.0
227.00	3927.0
228.00	536.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12

229.00	891.0
231.00	369.0
237.00	416.0
242.00	536.0
243.00	539.0
244.00	7949.0
245.00	1086.0
246.00	1470.0
255.00	42592.0
256.00	6072.0
256.90	477.0
258.00	2563.0
259.00	383.0
265.00	1040.0
273.00	1281.0
274.00	3452.0
275.00	20488.0
276.00	2673.0
277.00	1605.0
285.00	352.0
293.00	378.0
296.00	5761.0
297.00	803.0
303.00	771.0
314.00	313.0
315.00	686.0
316.00	395.0
323.00	1812.0
324.00	328.0
327.00	388.0
334.00	1342.0
335.00	305.0
346.00	492.0
352.00	579.0
352.90	462.0
354.00	721.0
365.00	2864.0
365.90	425.0
372.10	1097.0
383.00	330.0
402.00	423.0
403.00	676.0
421.00	571.0
422.00	600.0
423.00	4206.0
424.00	1092.0
441.10	10954.0
442.00	71984.0
443.00	13403.0
444.00	1204.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12

m/z	Abundance
39.90	780.0

Instrument :
BNA_N
ClientSampleId :
DFTPP12